

Certificate of Analysis

leil Beare

BDG Synthesis certifies that this reference material meets or exceeds the specifications stated herein.

Neil Beare, PhD, Director 8 January 2015

Efavirenz Name:

CAS Number: 154598-52-4

Structure:

 $C_{14}H_9ClF_3NO_2 = 315.68$ **Molecular Weight:**

BDG 4290 **Lot Number:**

Appearance: White, crystalline solid

Corrected Purity: 100.0 % (HPLC) - 0.2 % (excipients) = 99.8 %

Re-test Date: 8 January 2020

refrigerate for prolonged storage; may be handled and shipped at **Storage and Handling:** Temperature:

ambient temperature.

Humidity: not believed to be hygroscopic; may be handled in normal laboratory

atmosphere.

Light: protect from strong sunlight.

Caution: only experienced laboratory personnel should handle the material.

Version 4 (Id772) 1/5

Wellington, New Zealand.

• Custom synthesis of analytical reference standards, metabolites, stable isotope labelled compounds

Gracefield Research Centre, Building F,

• Contract research • BDG Synthesis is a division of B Dent Global Limited Phone: + 64 4 569 0520 info@bdg.co.nz

+ 6445690521www.bdg.co.nz

Identity and Purity

Proton NMR Spectrum

Identity: the signals are consistent with the proposed structure and in accord with literature where available. Residual Solvents: no residual solvents are observed.

Impurities: the small singlet at δ 1.19 is thought to arise from trace amounts of either magnesium stearate (64 methylene protons, M.W. = 591.27) or sodium lauryl sulfate (22 methylene protons, M.W. = 228.38). Integration of this signal suggests an upper bound of 0.2 % w/w (total amount for one or both materials).

Carbon-13 NMR Spectrum

Identity: the signals are consistent with the proposed structure and in accord with literature where available.

High-resolution Mass Spectrum (EI+)

Found *m/z* 315.0280. C₁₄H₉ClF₃NO₂ [M]⁺ requires *m/z* 315.0274. The deviation of 1.8 ppm is within normally accepted limits for the establishment of identity by HRMS.

HPLC

A sharp, symmetrical peak is observed (100.0 %). Note: in the absence of reference materials for preparing calibration curves, it is assumed that all peaks have the same detector response. Where possible, the conditions of analysis follow a pharmacopeial or literature method, or have been adapted from same.


Elemental Analysis

Found: C 53.30, H 2.73, N 4.53 % Requires: C 53.27, H 2.87, N 4.44 %


The elemental analyses fall within generally accepted limits for establishing the molecular formula given. The results may also be taken to imply the absence of significant quantities of water or inorganic salts (which have not been elsewhere tested for because of sample size limitations).


The available quantity of custom-synthesised material is always small, and this limits the extent and type of analytical data which can be obtained. This Certificate is presented in descriptive format for use by analytical chemists who are trained in the use of custom-synthesised materials. Custom materials often contain higher levels of residual solvents and/or water, and we urge you to use the corrected purity where needed rather than the raw HPLC purity. This compound is intended for use as an analytical reference material and it is not for human administration. Structures are shown with relative stereochemistry unless otherwise specified.

The re-test date is assigned from experience gained with the material in the laboratory and/or on storage. It is not possible to perform formal storage studies because of the small amount of material available.

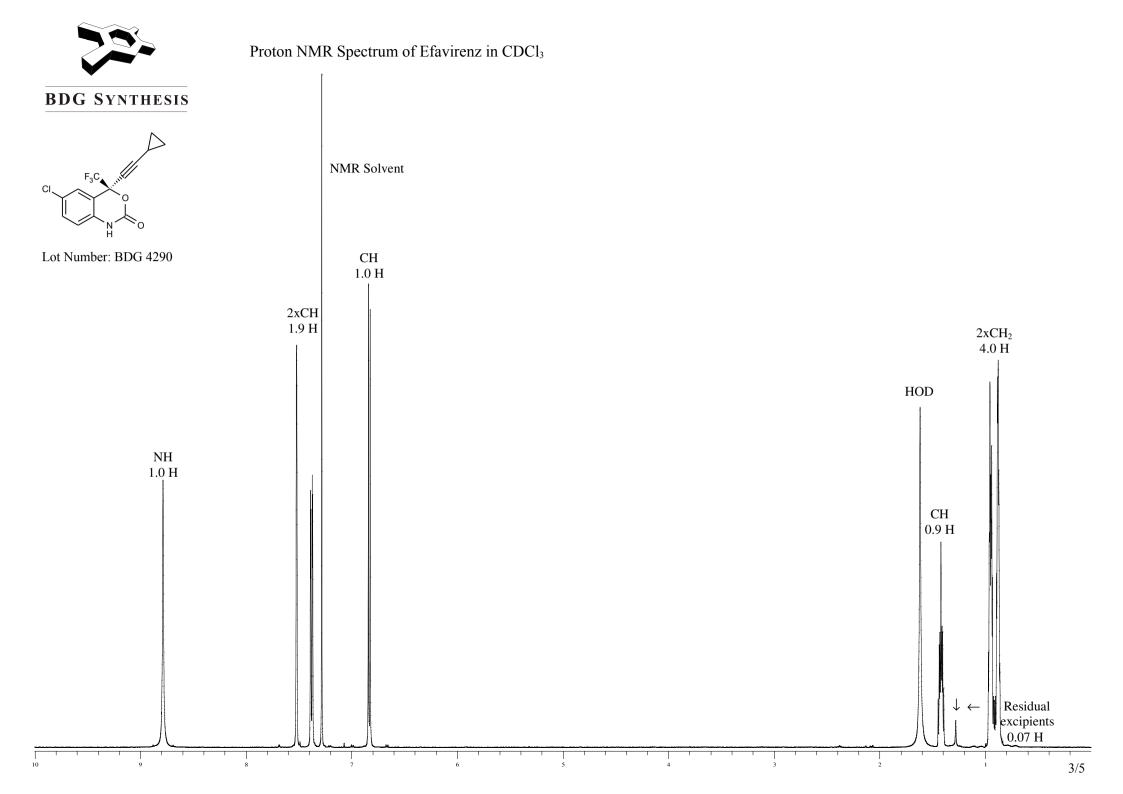





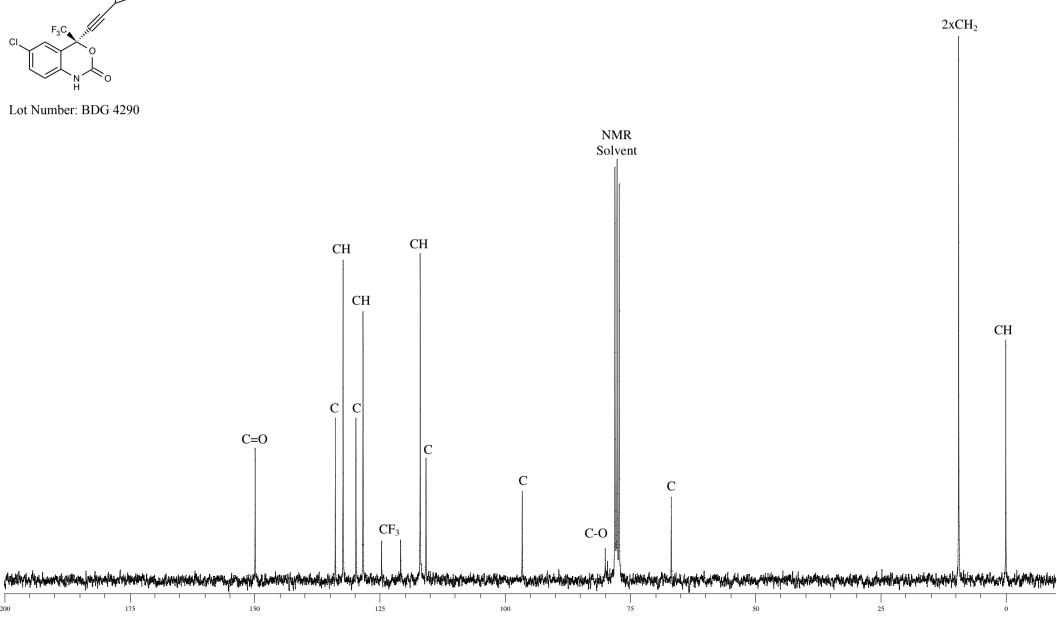

BDG - Analysis of Efavirenz

Column : Phenomenex Luna C18(2) 5um 250 x 4.6 mm Guard : Phenomenex Security Guard C18 RP 4 x 3 mm


Mobile Phase A: 50:50:0.05 Water: Acetonitrile: Trifluoroacetic Acid Mobile Phase B: 20:80:0.05 Water: Acetonitrile: Trifluoroacetic Acid Gradient (A:B): T0=100:0, T25=0:100, T30=0:100, T32=100:0, T35=100:0

Flow Rate: 1.0 mL/min

Sample Solvent: 1:1 Water: Acetonitrile

Column Temperature : 20C Injection Volume : 10 uL Detection : UV at 240 nm

| Sample Name | BDG 4290 | Instrument | AnalyticalLC01 |
|-------------|------------------------------|---------------|----------------|
| Acquisition | 08/01/2015, 13:16:09 | Method (rev.) | LC10259a (5) |
| Sequence | BDG_08Jan2014a - Reprocessed | Vial Position | 1 |
| Operator | solvation010\cerityadmin | Injection | 1 of 1 |

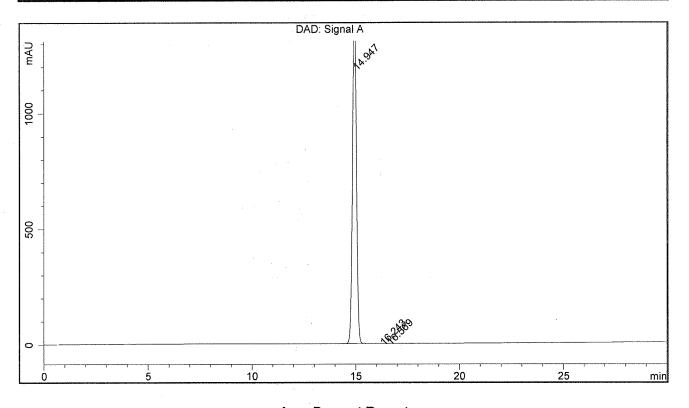

Area Percent Report

| Peak# | RT | Peak Height | Peak Area | Width | Area % |
|-------|-----------|-------------|------------|------------|----------|
| 1 | 14.95 min | 1541.4869 | 19328.2236 | 0.1923 min | 99.978 % |
| 2 | 16.24 min | 0.1704 | 1.4769 | 0.1151 min | 0.008 % |
| 3 | 16.57 min | 0.2320 | 2.8668 | 0.1701 min | 0.015 % |