



## BDG SYNTHESIS

### Certificate of Analysis

BDG Synthesis certifies that this reference material meets or exceeds the specifications stated herein.


*Barry Dent*

Barry R. Dent, PhD, Director  
1 April 2013

**Name:** Tetrazepam

**CAS Number:** 10379-14-3

**Structure:**



**Molecular Weight:**  $C_{16}H_{17}ClN_2O = 288.77$

**Lot Number:** BDG 1463

**Appearance:** Off-white, crystalline solid

**Purity By HPLC:** 99.7 %

**Re-test Date:** 1 April 2018

**Storage and Handling:**

Temperature:	refrigerate for prolonged storage; may be handled and shipped at ambient temperature.
Humidity:	not believed to be hygroscopic; may be handled in normal laboratory atmosphere.
Light:	protect from strong sunlight.
Caution:	only experienced laboratory personnel should handle the material.

## Identity and Purity

### Proton NMR Spectrum

Identity: the signals are consistent with the proposed structure and in accord with literature where available.

Residual Solvents: no residual solvents are observed.

Impurities: no significant impurities are evident in the spectrum.

### Carbon-13 NMR Spectrum

Identity: the signals are consistent with the proposed structure and in accord with literature where available.

### High-resolution Mass Spectrum (ESI+)

Found  $m/z$  311.0909.  $C_{16}H_{17}ClN_2ONa$   $[M+Na]^+$  requires  $m/z$  311.0922. The deviation of 4.0 ppm is within normally accepted limits for the establishment of identity by HRMS.

### HPLC

A sharp, symmetrical peak is observed (99.7 %). Note: in the absence of reference materials for preparing calibration curves, it is assumed that all peaks have the same detector response. Where possible, the conditions of analysis follow a pharmacopeial or literature method, or have been adapted from same.

### Elemental Analysis

$C_{16}H_{17}ClN_2O$	Found:	C 66.50, H 5.99, N 9.73 %
	Requires:	C 66.55, H 5.93, N 9.70 %

The elemental analyses fall within generally accepted limits for establishing the molecular formula given. The results may also be taken to imply the absence of significant quantities of water or inorganic salts (which have not been elsewhere tested for because of sample size limitations).


The available quantity of custom-synthesised material is always small, and this limits the extent and type of analytical data which can be obtained. This Certificate is presented in descriptive format for use by analytical chemists who are trained in the use of custom-synthesised materials. Custom materials often contain higher levels of residual solvents and/or water, and we urge you to use the corrected purity where needed rather than the raw HPLC purity. This compound is intended for use as an analytical reference material and it is not for human administration. Structures are shown with relative stereochemistry unless otherwise specified.

The re-test date is assigned from experience gained with the material in the laboratory and/or on storage. It is not possible to perform formal storage studies because of the small amount of material available.




# Proton NMR Spectrum of Tetrazepam in Methanol-d<sub>4</sub>

**BDG SYNTHESIS**




Lot Number: BDG 1463

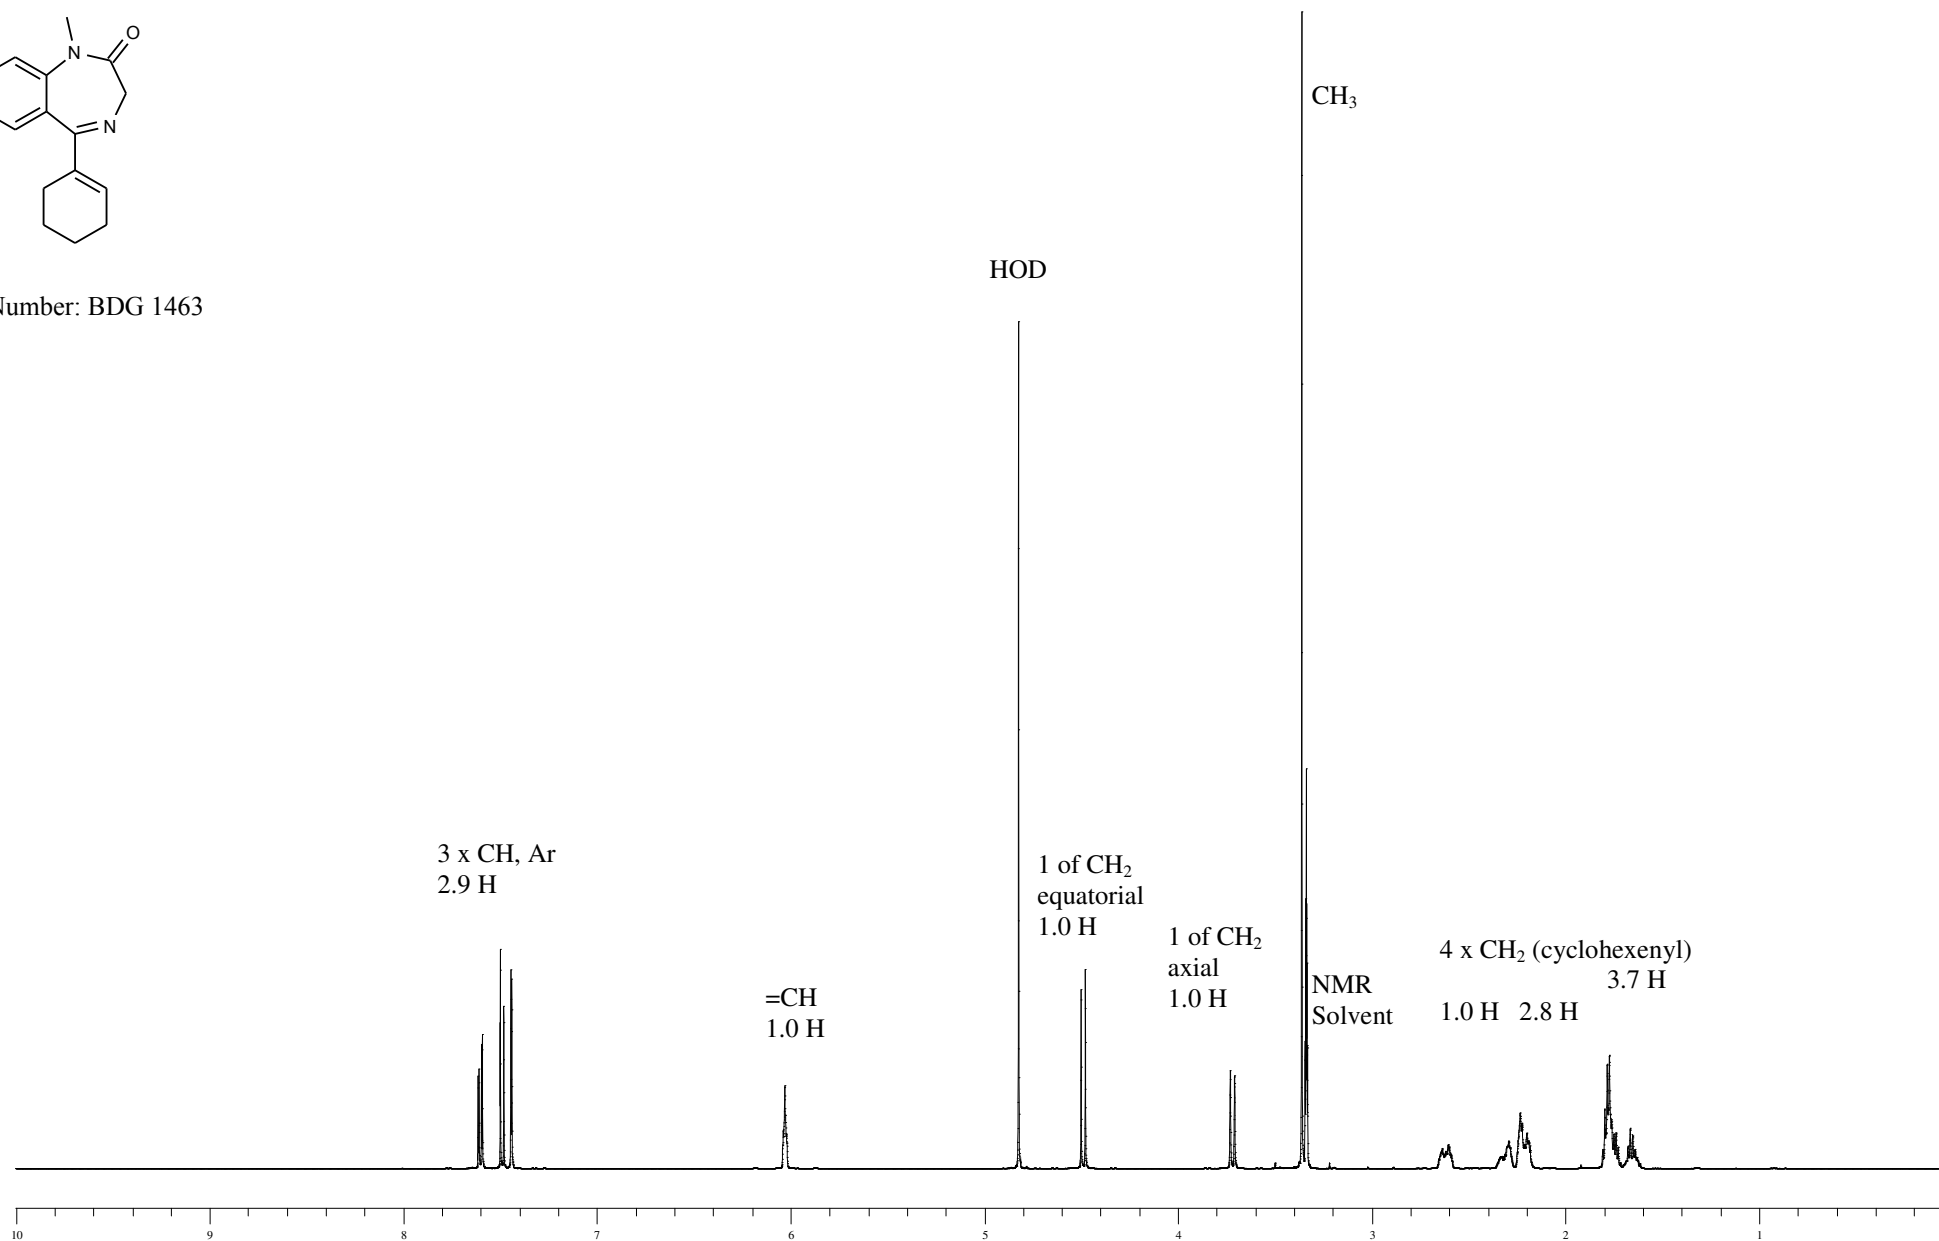




Carbon-13 NMR Spectrum of Tetrazepam in Methanol-d<sub>4</sub>

**BDG SYNTHESIS**




Lot Number: BDG 1463

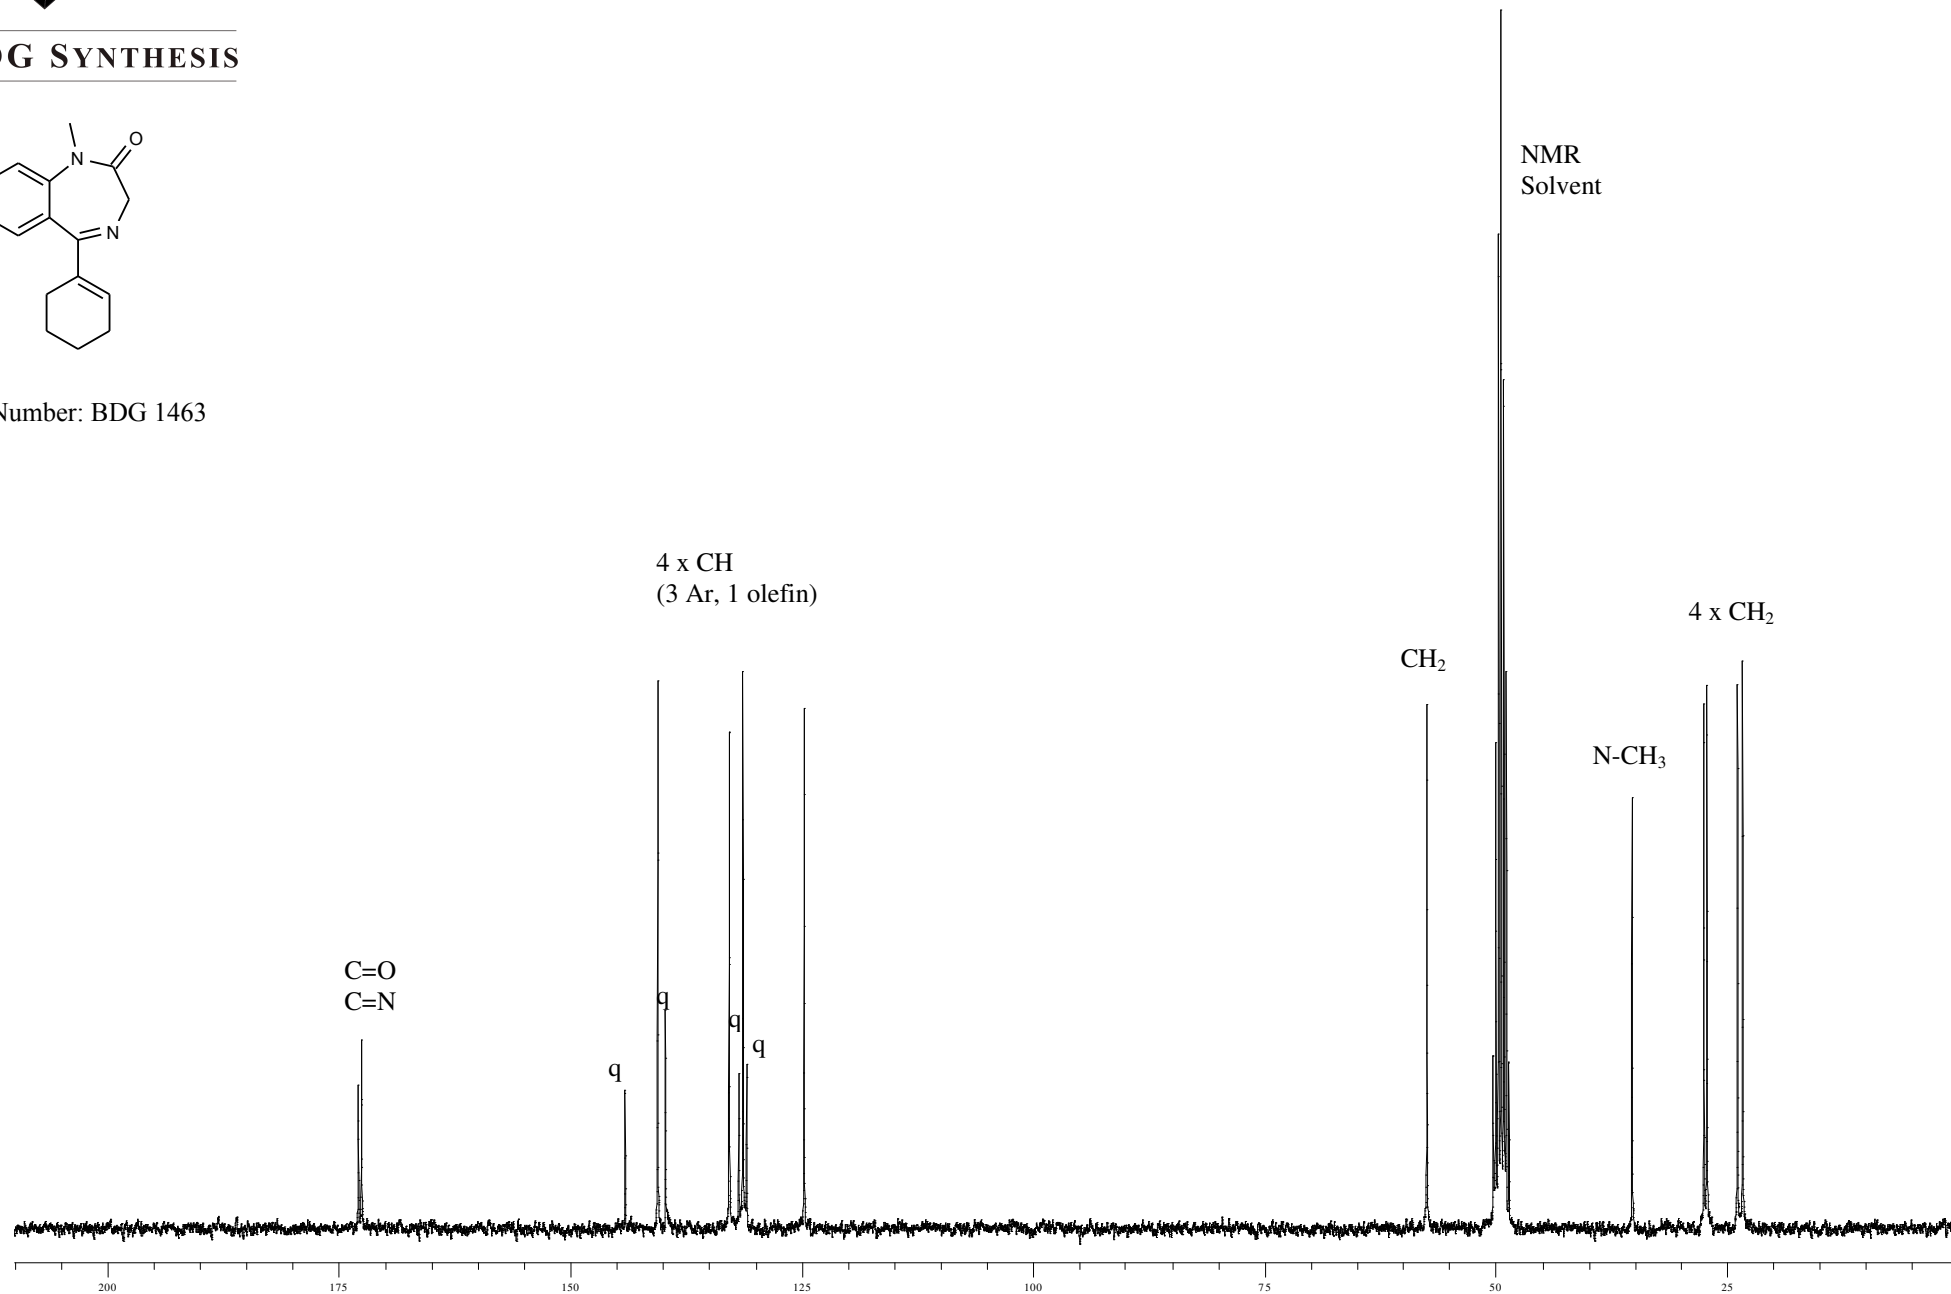

BDG - Analysis of Tetrazepam

Column : Phenomenex Luna C18(2) 5um 250 x 4.6 mm  
 Guard : Phenomenex Security Guard C18 RP 4 x 3 mm  
 Mobile Phase A : 60:40 25 mM Potassium diHydrogen Phosphate : Acetonitrile  
 Mobile Phase B : 33:67 25 mM Potassium diHydrogen Phosphate : Acetonitrile  
 Gradient : T0=100:0, T35=100:0, T40=0:100, T50=0:100, T55=100:0, T60=100:0  
 Flow Rate : 1.5 mL/min  
 Sample Solvent : 1:1 Water : Acetonitrile  
 Column Temperature : 20C  
 Injection Volume : 10 uL  
 Detection : UV at 229 nm

Sample Name	BDG 1463	Instrument	AnalyticalLC01
Acquisition	01/04/2013, 15:19:21	Method (rev.)	LC10303a ( 11 )
Sequence	BDG_01Apr2013c - Reprocessed	Vial Position	1
Operator	solvation010\cerityadmin	Injection	1 of 1

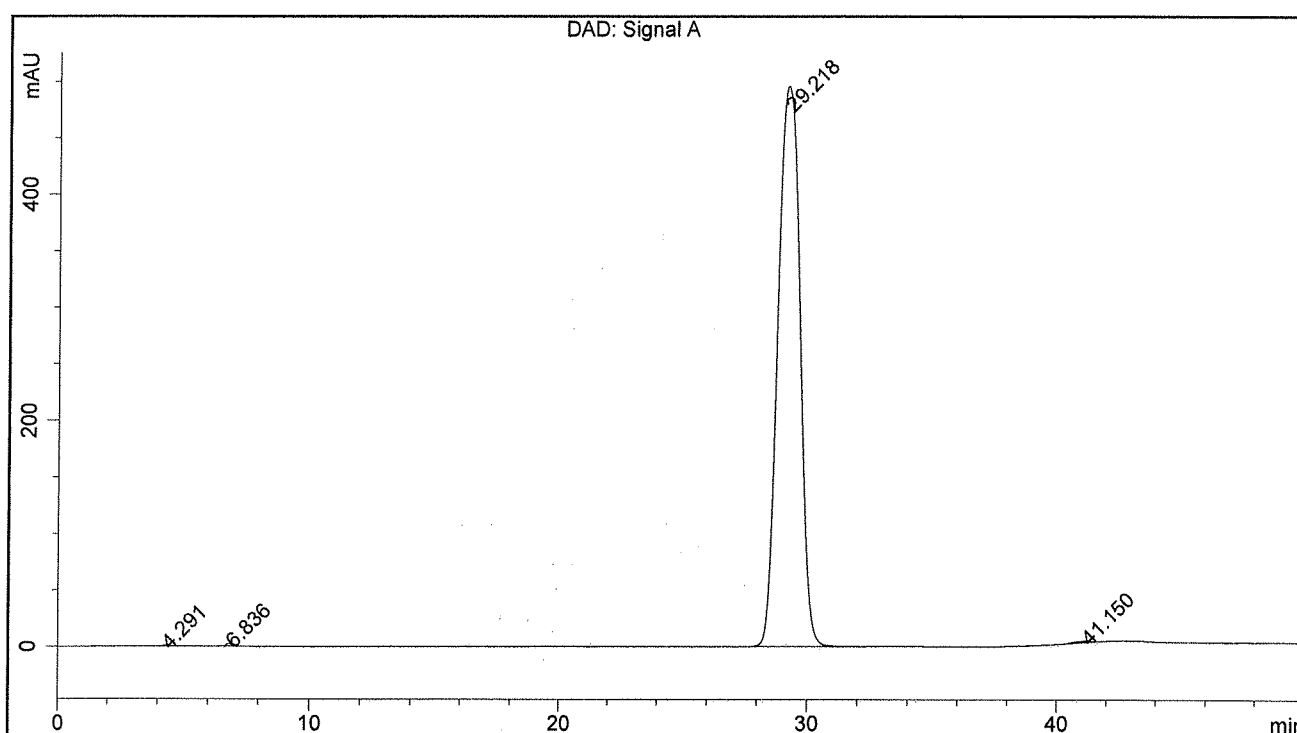

Area Percent Report

Peak#	RT	Peak Height	Peak Area	Width	Area %
1	4.29 min	0.6306	6.4869	0.1440 min	0.021 %
2	6.84 min	2.1443	31.4680	0.2392 min	0.103 %
3	29.22 min	495.3856	30355.2138	0.9949 min	99.699 %
4	41.15 min	1.2397	53.5732	0.5202 min	0.176 %