

BDG SYNTHESIS

Certificate of Analysis

BDG Synthesis certifies that this reference material meets or exceeds the specifications stated herein.


Neil Beare

Neil Beare, PhD, Director
6 July 2016

Name: Pioglitazone Ketone Metabolite

CAS Number: 146062-45-5

Structure:

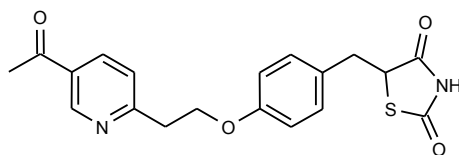

Molecular Weight: $C_{19}H_{18}N_2O_4S = 370.42$

Lot Number: BDG 10262.1

Appearance: White, crystalline solid

Corrected Purity: 98.6 % (HPLC) - 2.4 % (water) = 96.2 %

Re-test Date: 6 July 2021

Storage and Handling:

Temperature:	refrigerate for prolonged storage; may be handled and shipped at ambient temperature.
Humidity:	not believed to be hygroscopic; may be handled in normal laboratory atmosphere.
Light:	protect from strong sunlight.
Caution:	only experienced laboratory personnel should handle the material.

Identity and Purity

Proton NMR Spectrum

Identity: the signals are consistent with the proposed structure and in accord with literature where available.

Residual Solvents: no residual solvents are observed.

Impurities: no significant impurities are evident in the spectrum.

Carbon-13 NMR Spectrum

Identity: the signals are consistent with the proposed structure and in accord with literature where available.

High-resolution Mass Spectrum (ESI+)

Found m/z 393.0877. $C_{19}H_{18}N_2NaO_4S$ $[M+Na]^+$ requires m/z 393.0879. The deviation of 0.5 ppm is within normally accepted limits for the establishment of identity by HRMS.

HPLC

A sharp, symmetrical peak is observed (98.6 %). Note: in the absence of reference materials for preparing calibration curves, it is assumed that all peaks have the same detector response. Where possible, the conditions of analysis follow a pharmacopeial or literature method, or have been adapted from same.

Elemental Analysis

	Found:	C 60.49, H 4.81, N 7.40 %
$C_{19}H_{18}N_2O_4S \cdot 0.4H_2O$	Requires:	C 60.43, H 5.02, N 7.42 %
$C_{19}H_{18}N_2O_4S$	Requires:	C 61.61, H 4.90, N 7.56 %

The elemental analyses fall somewhat outside those expected for anhydrous material; the presence of water is reasonably expected from the method of purification and/or the type of material, and the "best-fit" hydrated molecular formula is given.

Karl-Fischer Analysis

	Found:	H ₂ O 2.4 %
$C_{19}H_{18}N_2O_4S \cdot 0.4H_2O$	Requires:	H ₂ O 1.9 %

Of necessity, only a small sample could be used and only a single or duplicate analysis performed. We are unable to state what the errors in the reported water content are, but recommend that the result be used, as the best available, when determining corrected purity.


The available quantity of custom-synthesised material is always small, and this limits the extent and type of analytical data which can be obtained. This Certificate is presented in descriptive format for use by analytical chemists who are trained in the use of custom-synthesised materials. Custom materials often contain higher levels of residual solvents and/or water, and we urge you to use the corrected purity where needed rather than the raw HPLC purity. This compound is intended for use as an analytical reference material and it is not for human administration. Structures are shown with relative stereochemistry unless otherwise specified.

The re-test date is assigned from experience gained with the material in the laboratory and/or on storage. It is not possible to perform formal storage studies because of the small amount of material available.




Proton NMR Spectrum of Pioglitazone Ketone Metabolite in DMSO-d₆

BDG SYNTHESIS

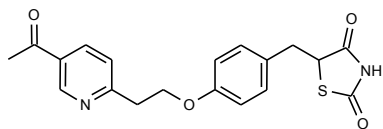


Lot Number: BDG 10262.1

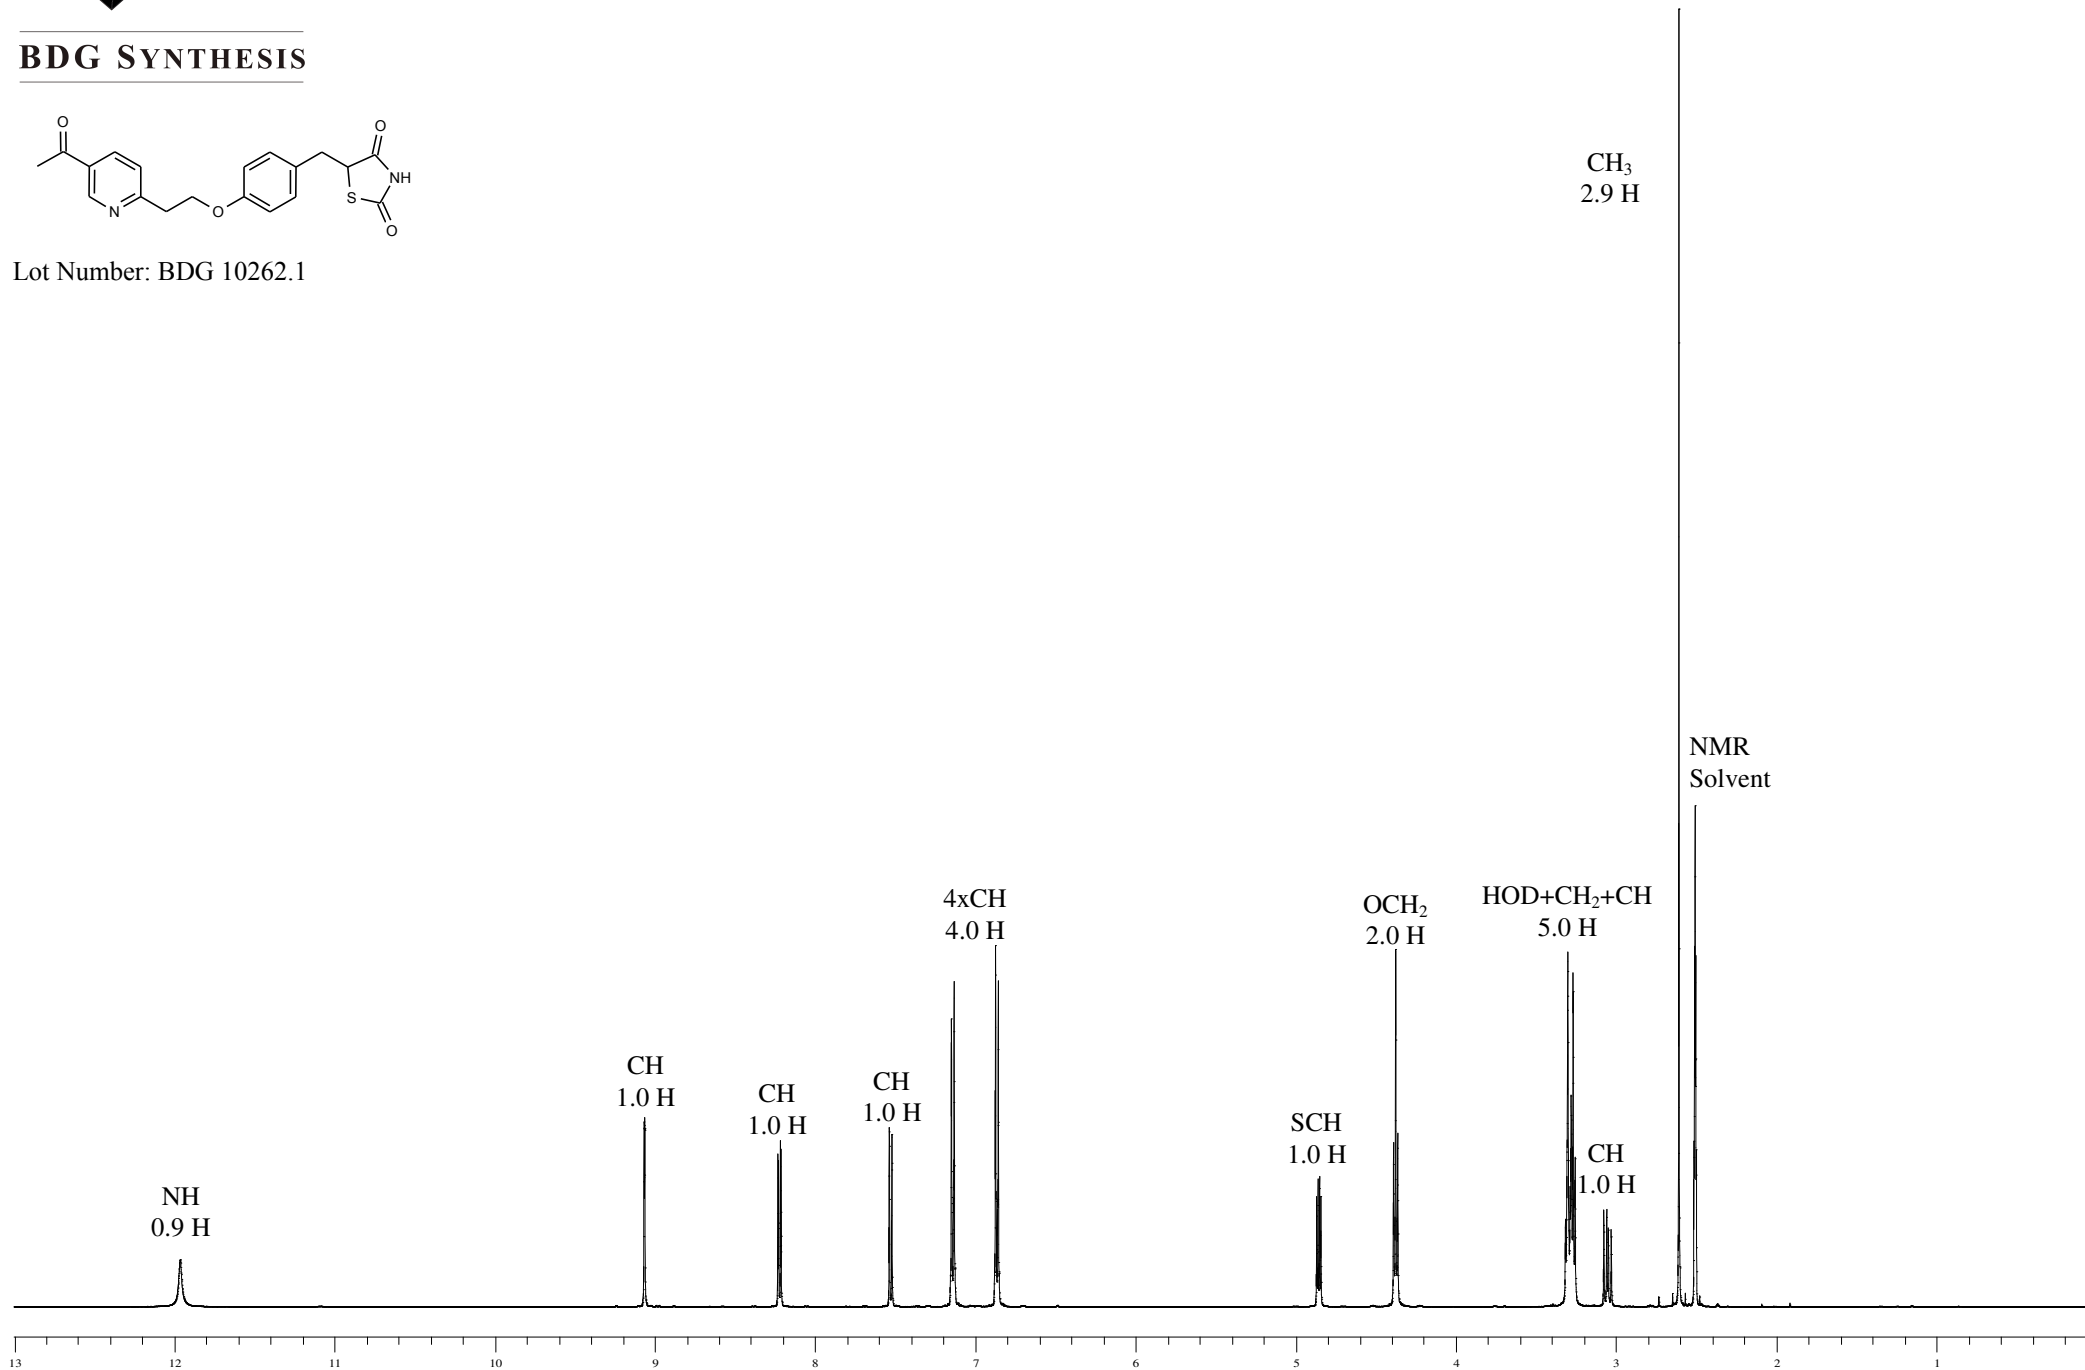




Carbon-13 NMR Spectrum of Pioglitazone Ketone Metabolite in DMSO-d₆

BDG SYNTHESIS

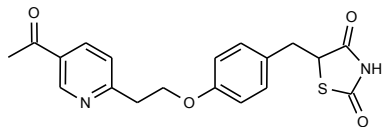


Lot Number: BDG 10262.1

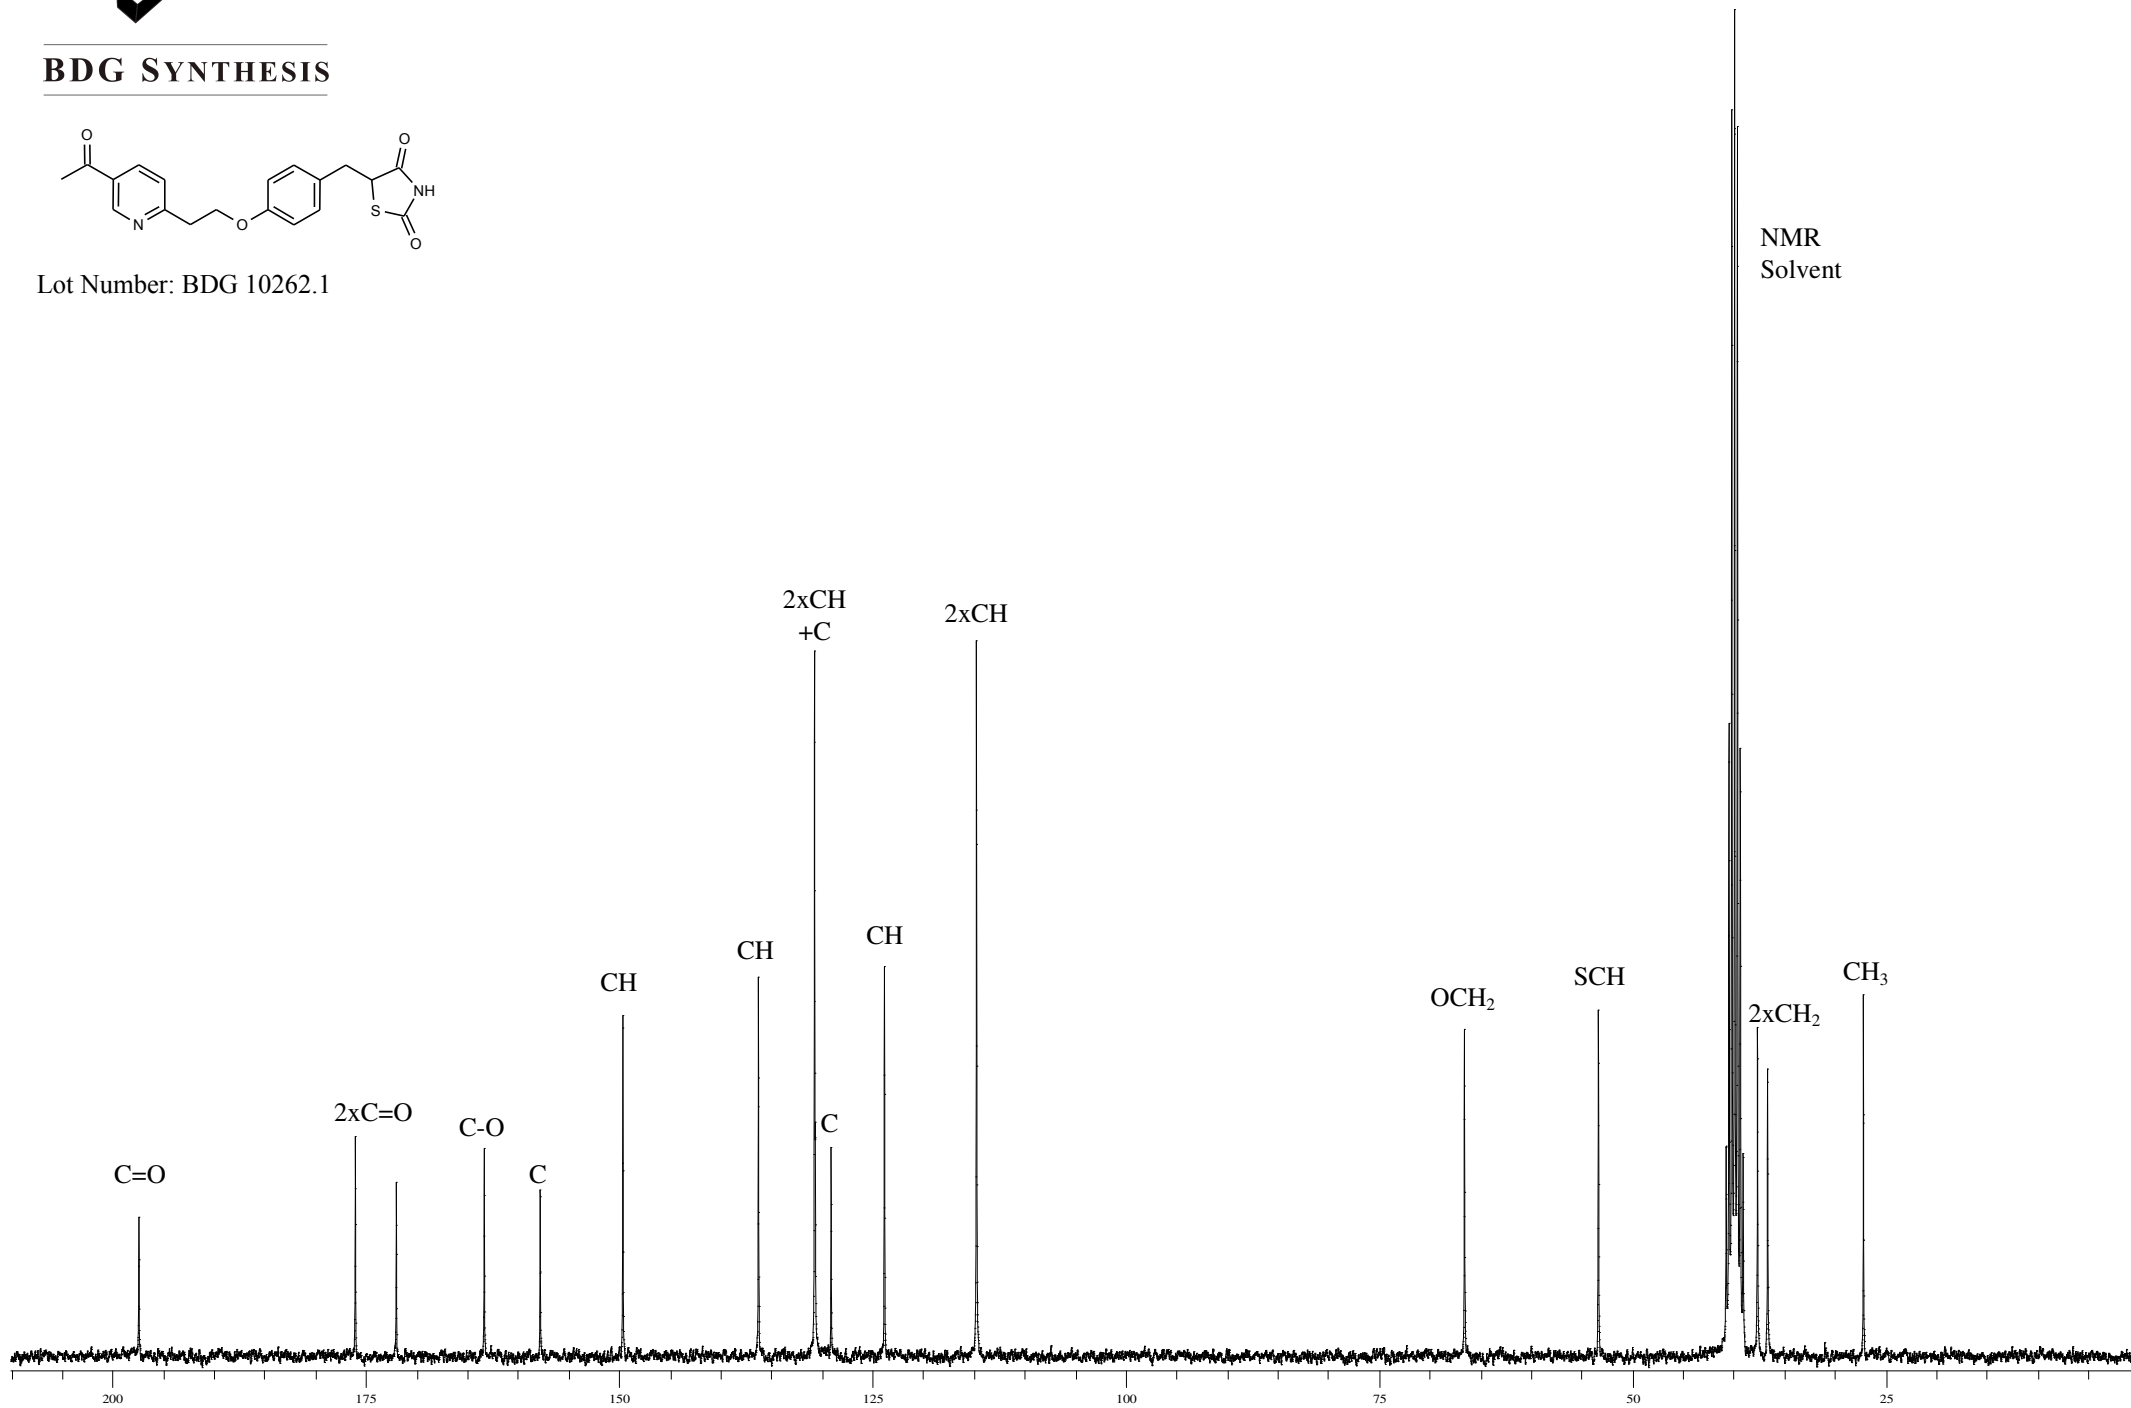

BDG - Analysis of Pioglitazone Ketone Metabolite

Column : Phenomenex Luna C18(2) 5um 250 x 4.6 mm
 Guard : Phenomenex Security Guard C18 RP 4 x 3 mm
 Mobile Phase : 65:35 10 mM Ammonium Acetate pH = 8.0 : Acetonitrile
 Flow Rate : 1 mL/min
 Sample Solvent : Mobile Phase
 Column Temperature : 50 C
 Injection Volume : 10 uL
 Detection : UV at 230 nm

Sample Name	BDG 10262.1	Instrument	AnalyticalLC01
Acquisition	06/07/2016, 17:21:03	Method (rev.)	LC10081c (5)
Sequence	BDG_06Jul2016a	Vial Position	25
Operator	solvation010\cerityadmin	Injection	2 of 2

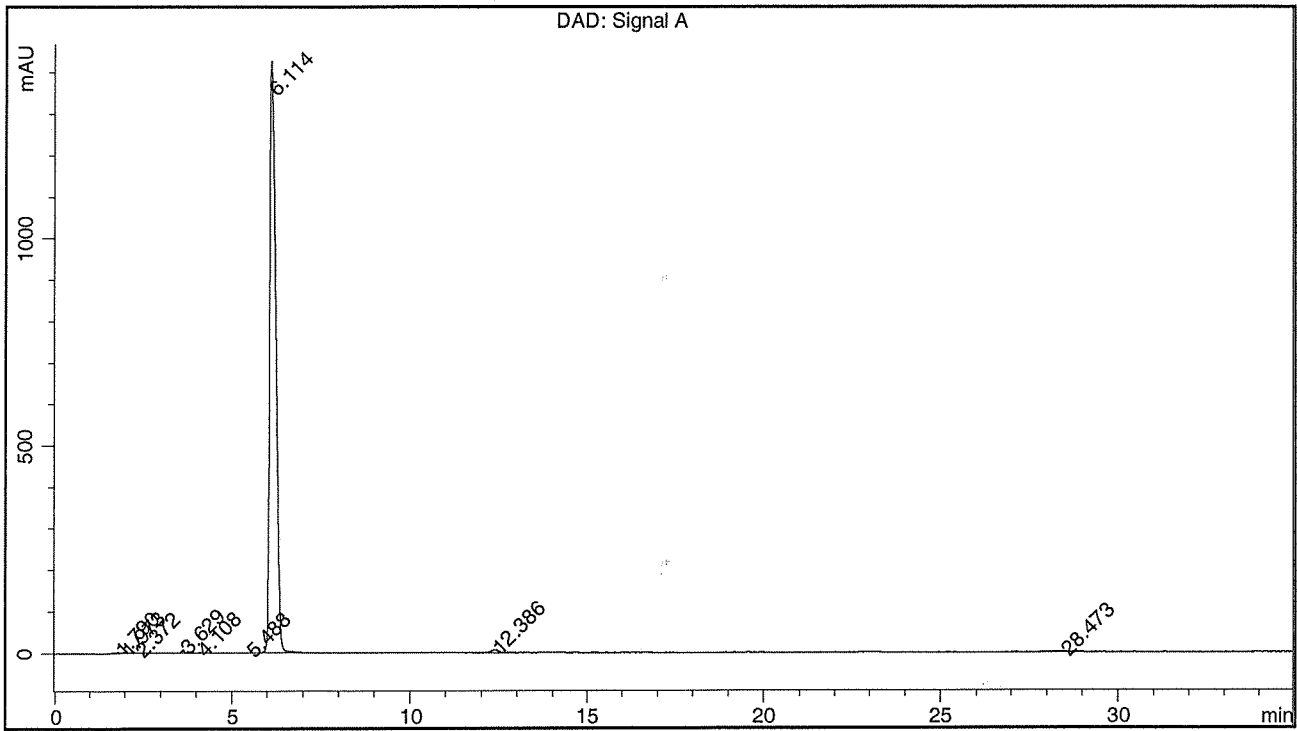

Area Percent Report

Peak#	RT	Peak Height	Peak Area	Width	Area %
1	1.79 min	1.8283	17.6971	0.1329 min	0.100 %
2	1.97 min	1.7545	25.2686	0.1900 min	0.143 %
3	2.37 min	0.9619	6.3279	0.0908 min	0.036 %
4	3.63 min	7.6005	41.2067	0.0853 min	0.234 %
5	4.11 min	1.5932	10.3882	0.1001 min	0.059 %
6	5.49 min	1.4851	11.9231	0.1197 min	0.068 %
7	6.11 min	1428.0547	17375.1249	0.1959 min	98.569 %
8	12.39 min	7.1740	106.4206	0.2271 min	0.604 %
9	28.47 min	1.0065	32.9319	0.3977 min	0.187 %