

# **Certificate of Analysis**

BDG Synthesis certifies that this reference material meets or exceeds the specifications stated herein.

Barry Dent

Barry R. Dent, PhD, Director 25 March 2014

Name: N-Methyl-4-pyridone-3-carboxamide

**CAS Number:** 769-49-3

Structure:

**Molecular Weight:**  $C_7H_8N_2O_2 = 152.15$ 

Lot Number: BDG 13281.3

**Appearance:** White, crystalline solid

**Corrected Purity:** 100.0 % (HPLC) - 5.1 % (water) = 94.9 %

**Re-test Date:** 25 March 2019

**Storage and Handling:** Temperature: refrigerate for prolonged storage; may be handled and shipped at

ambient temperature.

Humidity: not believed to be hygroscopic; may be handled in normal laboratory

atmosphere.

Light: protect from strong sunlight.

Caution: only experienced laboratory personnel should handle the material.

Phone: + 64 4 569 0520 Fax: + 64 4 569 0521 info@bdg.co.nz www.bdg.co.nz

### **Identity and Purity**

### **Proton NMR Spectrum**

Identity: the signals are consistent with the proposed structure and in accord with literature where available.

Residual Solvents: no residual solvents are observed.

Impurities: no significant impurities are evident in the spectrum.

#### **Carbon-13 NMR Spectrum**

Identity: the signals are consistent with the proposed structure and in accord with literature where available.

#### **High-resolution Mass Spectrum (ESI+)**

Found *m/z* 175.0480. C<sub>7</sub>H<sub>8</sub>N<sub>2</sub>NaO<sub>2</sub> [M+Na]<sup>+</sup> requires *m/z* 175.0483. The deviation of 1.7 ppm is within normally accepted limits for the establishment of identity by HRMS.

#### **HPLC**

A sharp, slightly tailing peak is observed (100.0 %). Note: in the absence of reference materials for preparing calibration curves, it is assumed that all peaks have the same detector response. Where possible, the conditions of analysis follow a pharmacopeial or literature method, or have been adapted from same.

#### **Elemental Analysis**

Found: C 52.43, H 5.68, N 17.43 %

 $C_7H_8N_2O_2\cdot 0.4H_2O$  Requires: C 52.76, H 5.57, N 17.58 %  $C_7H_8N_2O_2$  Requires: C 55.26, H 5.30, N 18.41 %

The elemental analyses fall substantially outside those expected for anhydrous material; the presence of water is reasonably expected from the method of purification and/or the type of material, and the "best-fit" hydrated molecular formula is given.

#### **Karl-Fischer Analysis**

Found: H<sub>2</sub>O 5.1 %

 $C_7H_8N_2O_2\cdot 0.4H_2O$  Requires:  $H_2O 4.5 \%$ 


Of necessity, only a small sample could be used and only a single or duplicate analysis performed. We are unable to state what the errors in the reported water content are, but recommend that the result be used, as the best available, when determining corrected purity.

The available quantity of custom-synthesised material is always small, and this limits the extent and type of analytical data which can be obtained. This Certificate is presented in descriptive format for use by analytical chemists who are trained in the use of custom-synthesised materials. Custom materials often contain higher levels of residual solvents and/or water, and we urge you to use the corrected purity where needed rather than the raw HPLC purity. This compound is intended for use as an analytical reference material and it is not for human administration. Structures are shown with relative stereochemistry unless otherwise specified.

The re-test date is assigned from experience gained with the material in the laboratory and/or on storage. It is not possible to perform formal storage studies because of the small amount of material available.

CH 0.9 H

# **BDG SYNTHESIS**



Lot Number: BDG 13281.3

NH


1.0 H

СН 1.0 H

CH 1.0 H


NH


1.0 H

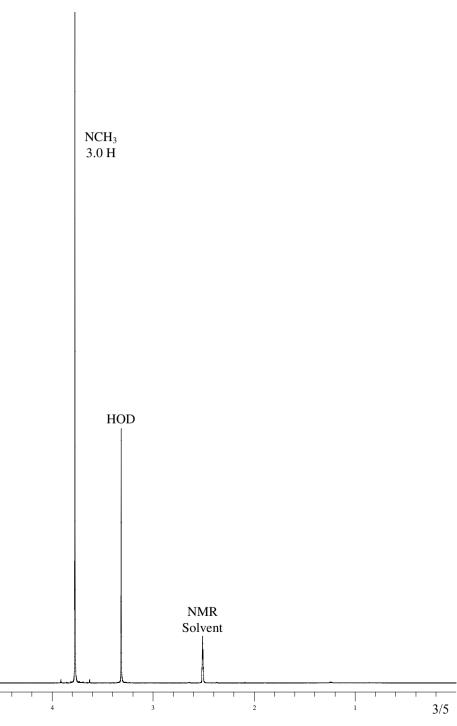



# **BDG SYNTHESIS**



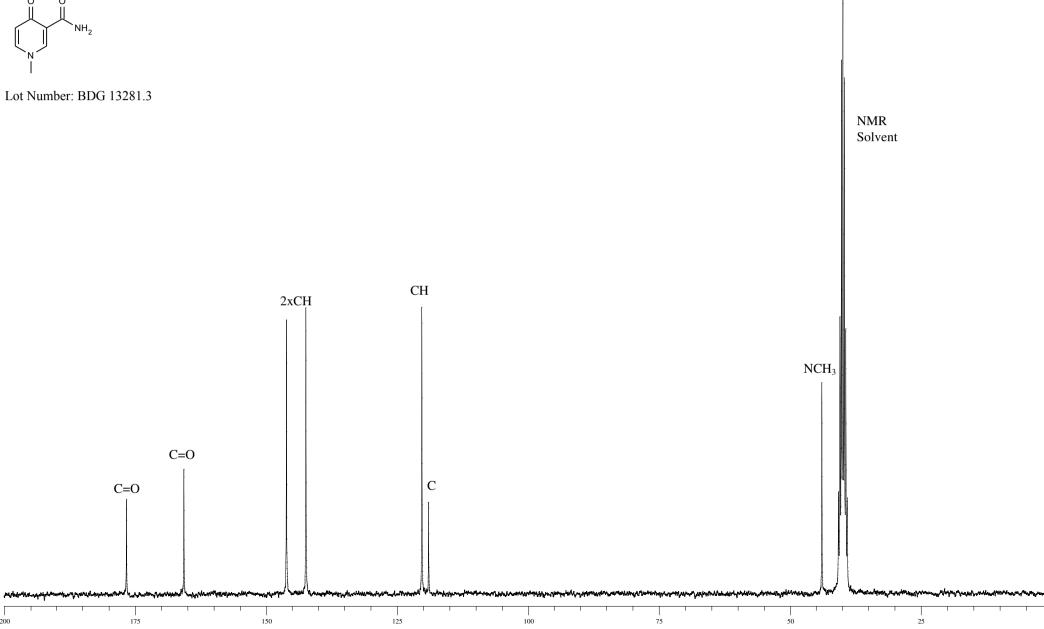


BDG - Analysis of N-Methyl-4-pyridone-3-carboxamide

Column : Phenomenex Luna C18(2) 5um 250 x 4.6 mm Guard : Phenomenex Security Guard C18 RP 4 x 3 mm Mobile Phase : 96:4:0.05 Water : Acetonitrile : Acetic Acid

Flow Rate: 1.0 mL/min

Sample Solvent : Mobile Phase Column Temperature : 20C Injection Volume : 10 uL Detection : UV at 254 nm

Sample Name	BDG 13281.3	Instrument	AnalyticalLC01
Acquisition	25/03/2014, 12:31:46	Method (rev.)	LC10284c (7)
Sequence	BDG_25Mar2014a - Reprocessed	Vial Position	21
Operator	solvation010\cerityadmin	Injection	2 of 2

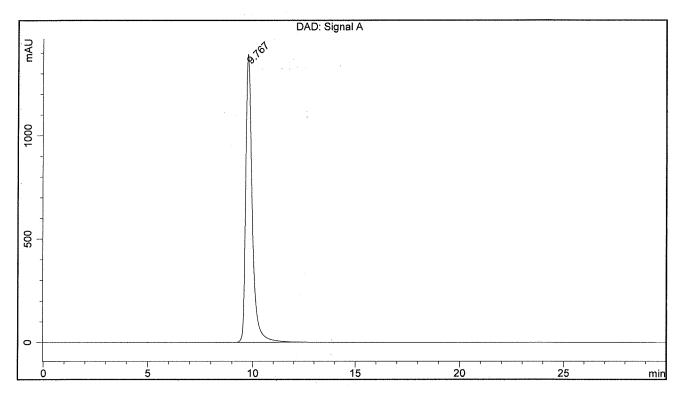

### **Area Percent Report**

Peak#	RT	Peak Height	Peak Area	Width	Area %
1	9.77 min	1392.5227	30870.1397	0.3326 min	100.000 %