



## BDG SYNTHESIS

### Certificate of Analysis

BDG Synthesis certifies that this reference material meets or exceeds the specifications stated herein.


*Barry Dent*

Barry R. Dent, PhD, Director  
15 February 2014

**Name:** Methotrimeprazine-d<sub>3</sub> Maleate

**CAS Number:** 60-99-1 (unlabelled)

**Structure:**

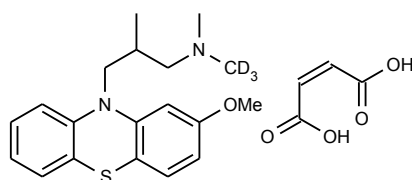

**Molecular Weight:** C<sub>19</sub>H<sub>21</sub>D<sub>3</sub>N<sub>2</sub>OS·C<sub>4</sub>H<sub>4</sub>O<sub>4</sub> = 447.56

**Lot Number:** BDG 1471

**Appearance:** White, crystalline solid

**Purity By HPLC:** 99.6 %

**Isotopic Purity:** Under 0.5 % d<sub>0</sub>

**Re-test Date:** 15 February 2019

**Storage and Handling:**

Temperature:	refrigerate for prolonged storage; may be handled and shipped at ambient temperature.
Humidity:	not believed to be hygroscopic; may be handled in normal laboratory atmosphere.
Light:	store in an amber vial and protect from bright light.
Caution:	only experienced laboratory personnel should handle the material.

## Identity and Purity

### Proton NMR Spectrum

Identity: the signals are consistent with the proposed structure and in accord with literature where available.

Isotopic Labelling: signals at the site of deuteration are absent, compared with what would be expected for unlabelled material, indicating clean deuteration.

Residual Solvents: no residual solvents are observed.

Impurities: no significant impurities are evident in the spectrum.

### Carbon-13 NMR Spectrum

Identity: the signals are consistent with the proposed structure and in accord with literature where available.

Isotopic Labelling: signals at the site of deuteration have collapsed to small multiplets compared with what would be expected for unlabelled material, indicating clean deuteration.

### High-resolution Mass Spectrum (ESI+)

Found  $m/z$  332.1872.  $C_{19}H_{22}D_3N_2OS$   $[M+H]^+$  requires  $m/z$  332.1876. The deviation of 1.2 ppm is within normally accepted limits for the establishment of identity by HRMS. No signal for  $d_0$  material was seen (detection limit about 0.5 %).

### HPLC

A sharp, symmetrical peak is observed (99.6 %). Note: in the absence of reference materials for preparing calibration curves, it is assumed that all peaks have the same detector response. Where possible, the conditions of analysis follow a pharmacopeial or literature method, or have been adapted from same.

### Elemental Analysis

	Found:	C 61.90, H 5.61, D 1.36, N 6.29 %
$C_{19}H_{21}D_3N_2OS \cdot C_4H_4O_4$	Requires:	C 61.72, H 5.63, D 1.35, N 6.26 %

The elemental analyses fall within generally accepted limits for establishing the molecular formula given. The results may also be taken to imply the absence of significant quantities of water or inorganic salts (which have not been elsewhere tested for because of sample size limitations).


The available quantity of custom-synthesised material is always small, and this limits the extent and type of analytical data which can be obtained. This Certificate is presented in descriptive format for use by analytical chemists who are trained in the use of custom-synthesised materials. Custom materials often contain higher levels of residual solvents and/or water, and we urge you to use the corrected purity where needed rather than the raw HPLC purity. This compound is intended for use as an analytical reference material and it is not for human administration. Structures are shown with relative stereochemistry unless otherwise specified.

The re-test date is assigned from experience gained with the material in the laboratory and/or on storage. It is not possible to perform formal storage studies because of the small amount of material available.




Proton NMR Spectrum of Methotrimeprazine-d<sub>3</sub> Maleate in DMSO-d<sub>6</sub>

**BDG SYNTHESIS**

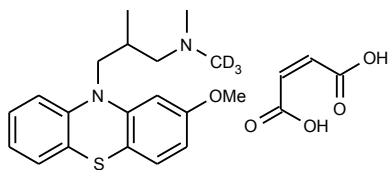


Lot Number: BDG 1471

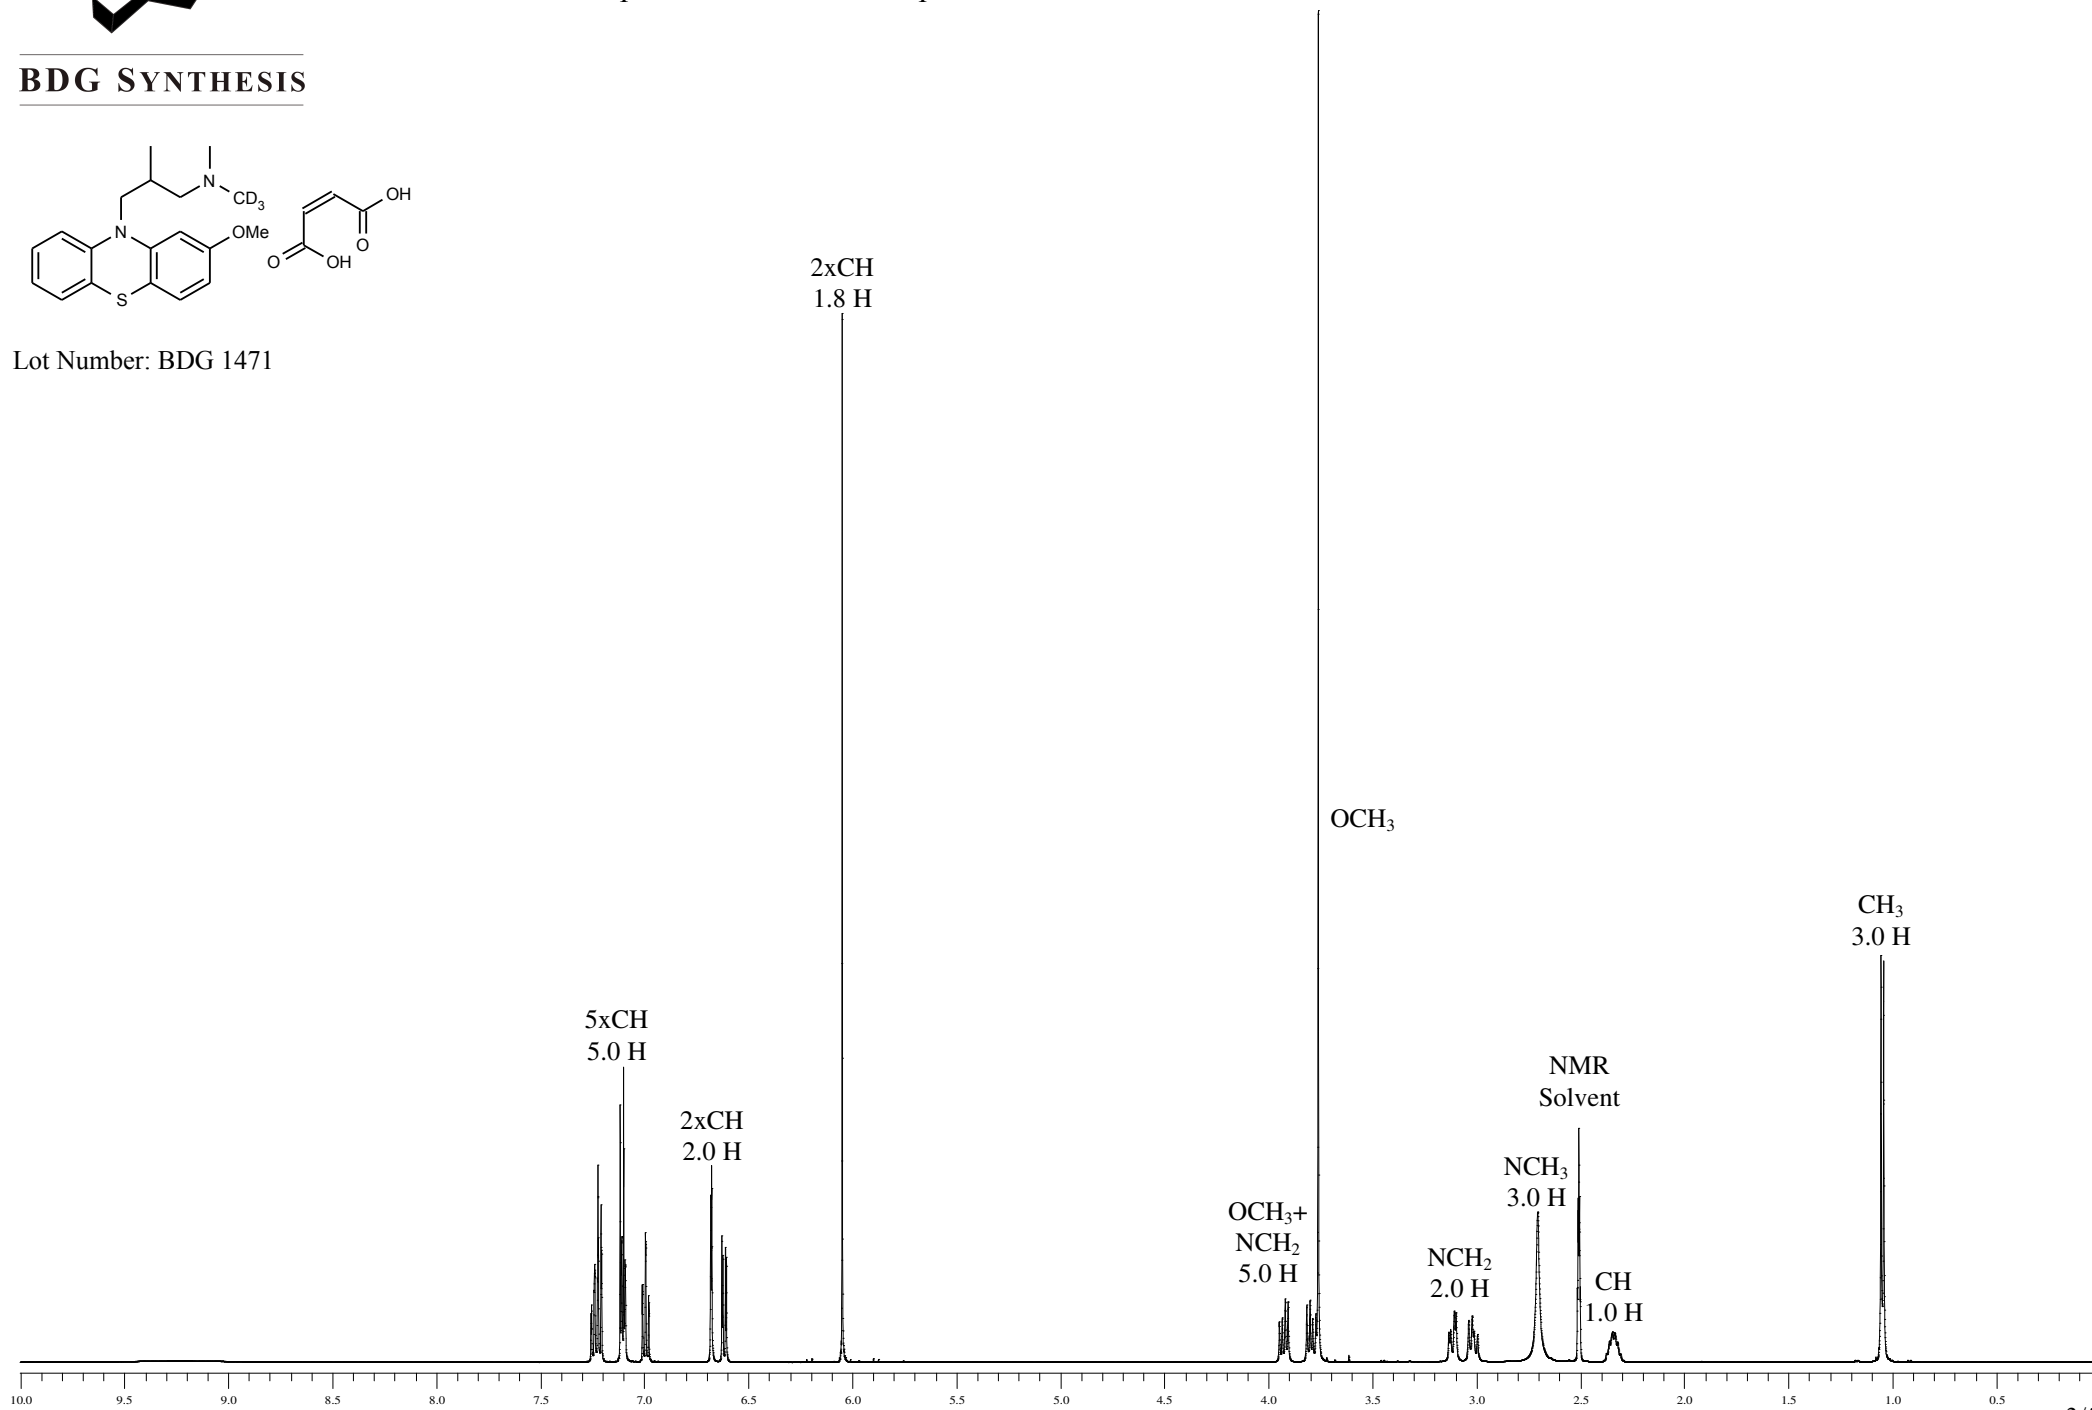




# Carbon-13 NMR Spectrum of Methotrimeprazine-d<sub>3</sub> Maleate in DMSO-d<sub>6</sub>

## BDG SYNTHESIS

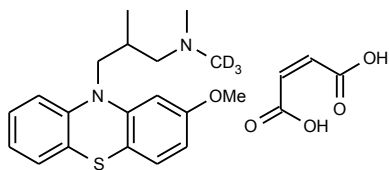


Lot Number: BDG 1471

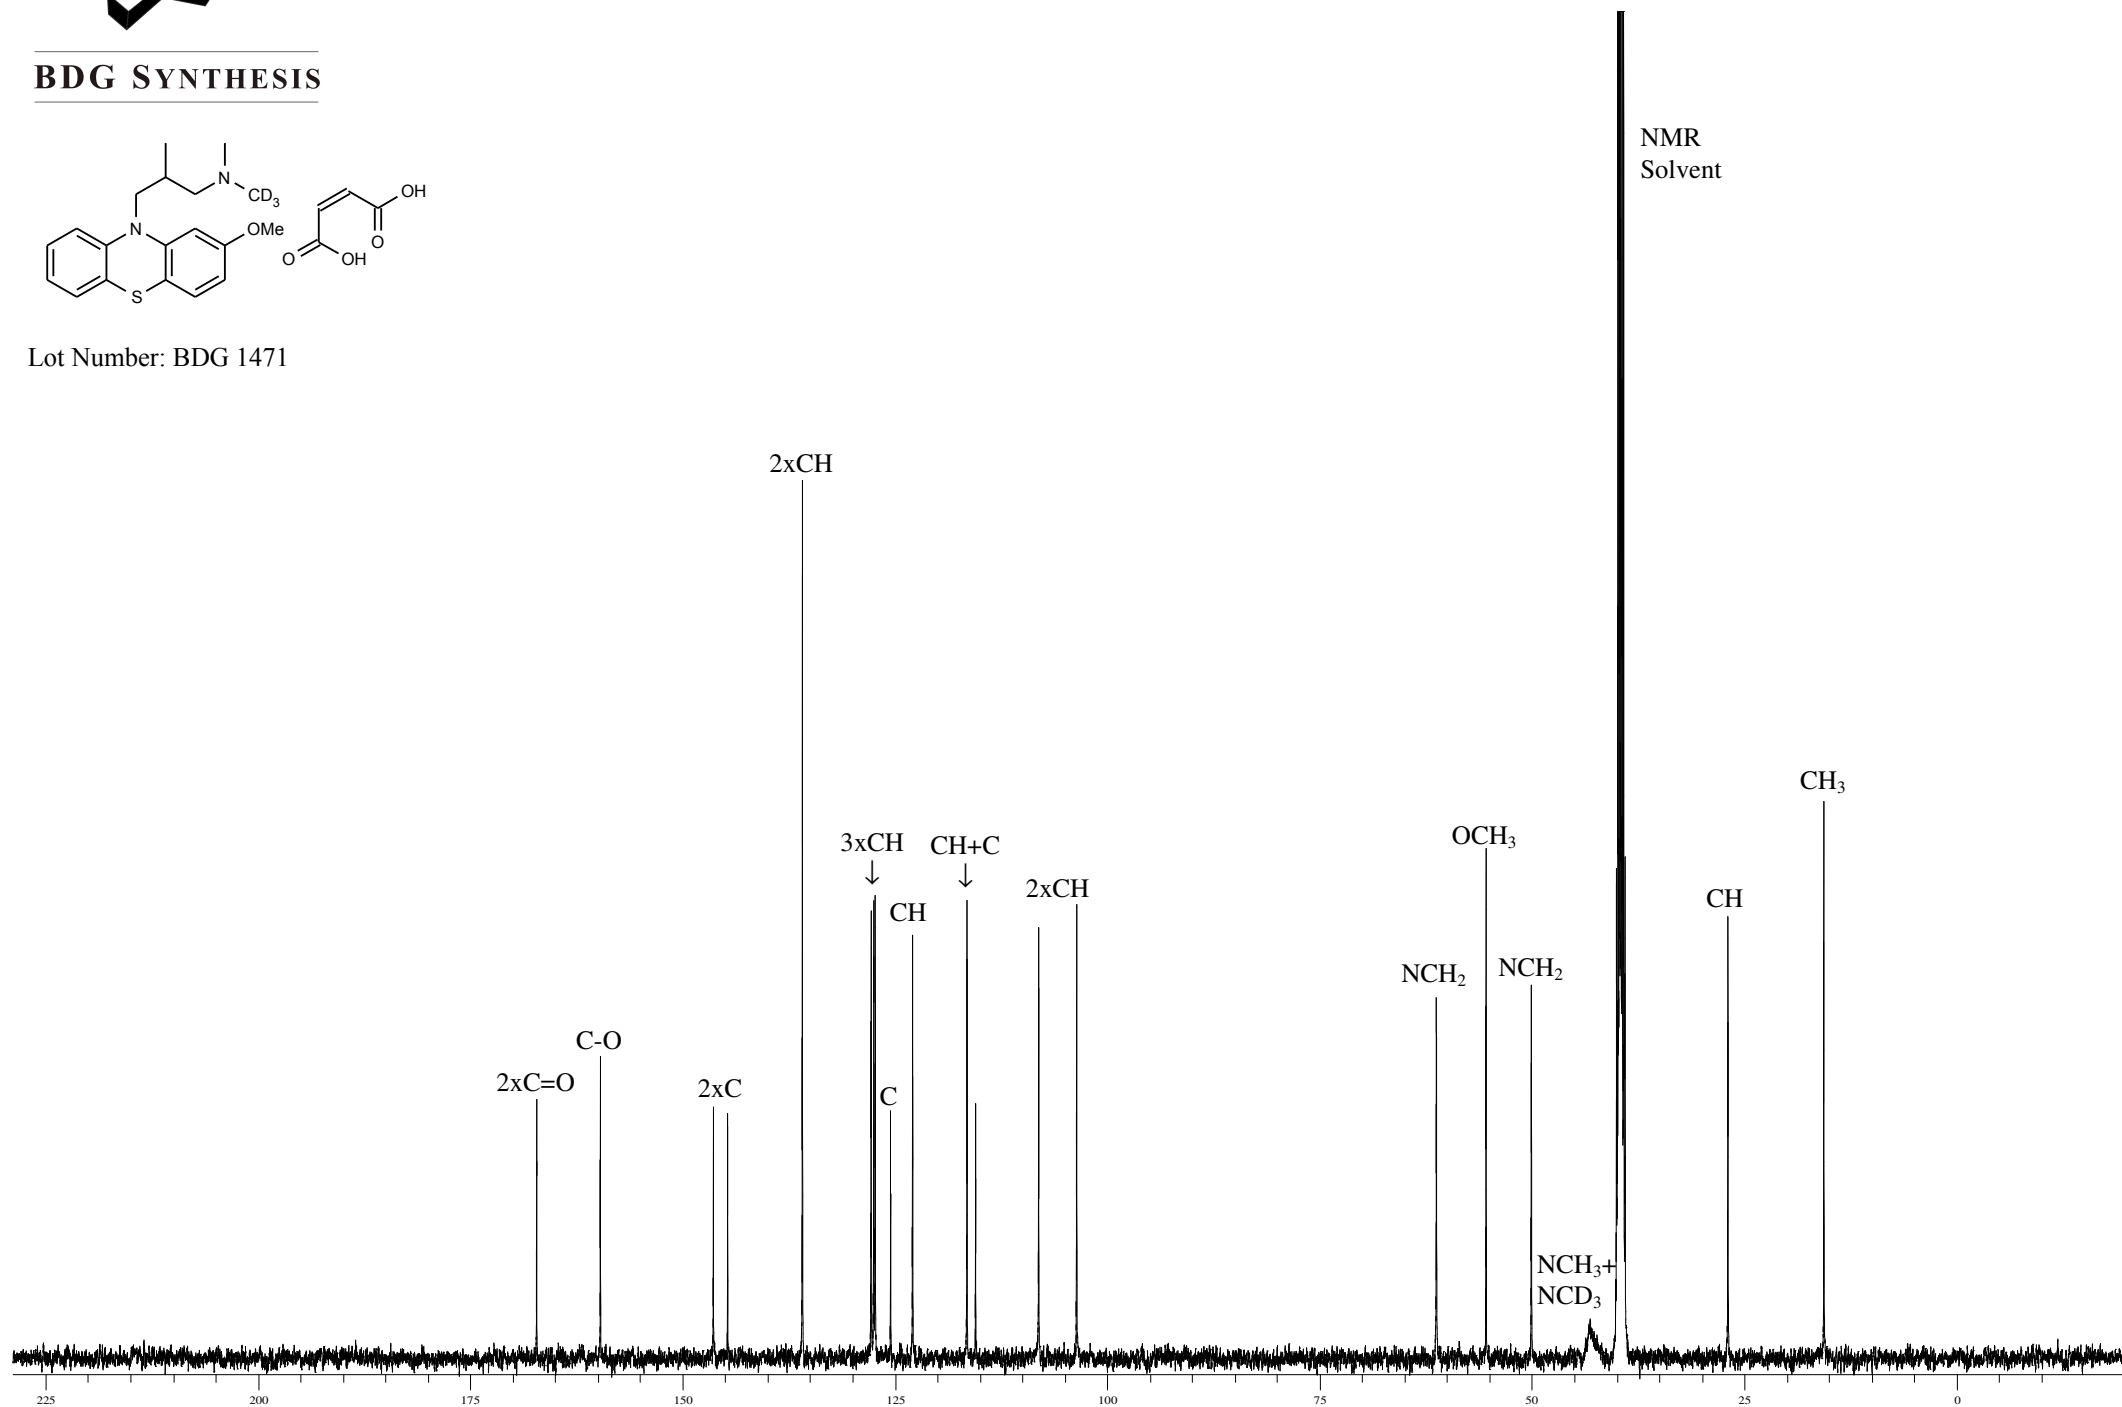

BDG - Analysis of Methotrimeprazine-d3 Maleate

Column : Phenomenex Luna C18(2) 5um 250 x 4.6 mm  
 Guard : Phenomenex Security Guard C18 4 x 3 mm  
 Mobile Phase A : 75:25:0.1 Water : Acetonitrile : Trifluoroacetic Acid  
 Mobile Phase B : 30:70:0.1 Water : Acetonitrile : Trifluoroacetic Acid  
 Gradient (A:B) : T0=100:0, T20=0:100, T24=0:100, T27=100:0, T30=100:0  
 Flow Rate : 1.0 mL/min  
 Sample Solvent : 70:30 Water : Acetonitrile  
 Column Temperature : 20C  
 Injection Volume : 10 uL  
 Detection : UV at 250 nm

<b>Sample Name</b>	BDG 1471	<b>Instrument</b>	AnalyticalLC01
<b>Acquisition</b>	15/02/2014, 12:08:19	<b>Method (rev.)</b>	LC10290c ( 4 )
<b>Sequence</b>	BDG_15Feb2014a - Reprocessed	<b>Vial Position</b>	6
<b>Operator</b>	solvation010\cerityadmin	<b>Injection</b>	1 of 1

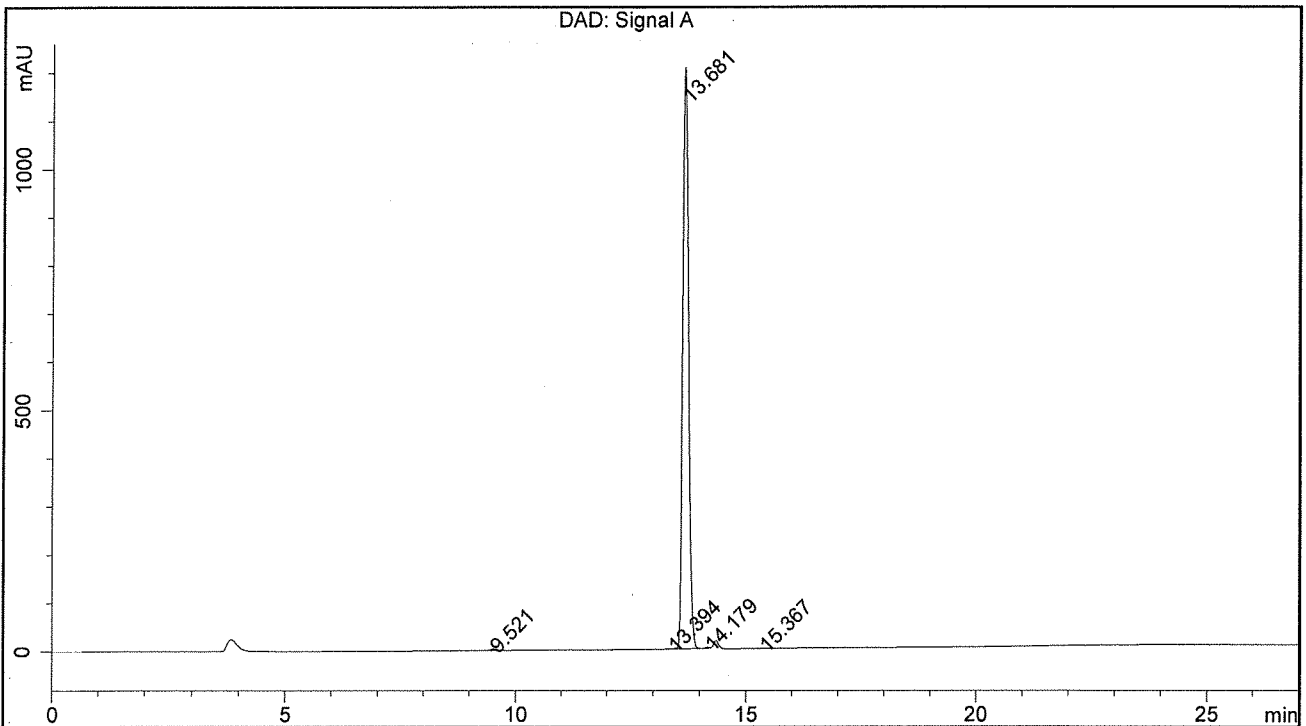

Area Percent Report

Peak#	RT	Peak Height	Peak Area	Width	Area %
1	9.52 min	2.9490	25.4680	0.1208 min	0.241 %
2	13.39 min	0.9320	8.1084	0.1235 min	0.077 %
3	13.68 min	1205.5228	10544.2649	0.1380 min	99.573 %
4	14.18 min	1.6738	7.7184	0.0758 min	0.073 %
5	15.37 min	0.5268	3.8830	0.1100 min	0.037 %