



BDG SYNTHESIS

Certificate of Analysis


BDG Synthesis certifies that this reference material meets or exceeds the specifications stated herein.

Barry Dent

Barry R. Dent, PhD, Director
23 July 2013

Name: Memantine-d₆ HCl
CAS Number: 41100-52-1 (unlabelled)

Structure:



Molecular Weight: C₁₂H₁₅D₆N·HCl = 221.80
Lot Number: BDG 13810
Appearance: White, crystalline solid
Corrected Purity: 99.1 % (HPLC) - 0.3 % (2-propanol) - 3.9 % (water) = 94.9 %
Isotopic Purity: Under 0.5 % d₀
Re-test Date: 23 July 2018

Storage and Handling: Temperature: refrigerate for prolonged storage; may be handled and shipped at ambient temperature.
Humidity: not believed to be hygroscopic; may be handled in normal laboratory atmosphere.
Light: protect from strong sunlight.
Caution: only experienced laboratory personnel should handle the material.

Identity and Purity

Proton NMR Spectrum

Identity: the signals are consistent with the proposed structure and in accord with literature where available.

Isotopic Labelling: signals at the sites of deuteration are greatly diminished, compared with what would be expected for unlabelled material, indicating clean deuteration.

Residual Solvents: a small amount of 2-propanol (0.3 % w/w) is observed.

Impurities: no significant impurities are evident in the spectrum.

Carbon-13 NMR Spectrum

Identity: the signals are consistent with the proposed structure and in accord with literature where available.

Isotopic Labelling: signals at the sites of deuteration have collapsed to small multiplets compared with what would be expected for unlabelled material, indicating clean deuteration.

High-resolution Mass Spectrum (ESI+)

Found m/z 186.2123. $C_{12}H_{16}D_6N$ $[M+H]^+$ requires m/z 186.2129. The deviation of 3.2 ppm is within normally accepted limits for the establishment of identity by HRMS. No signal for d_0 material was seen (detection limit about 0.5 %).

HPLC

A sharp, symmetrical peak is observed (99.1 %). Note: in the absence of reference materials for preparing calibration curves, it is assumed that all peaks have the same detector response. Where possible, the conditions of analysis follow a pharmacopeial or literature method, or have been adapted from same.

Elemental Analysis

	Found:	C 62.41, H 7.15, D 5.36, N 6.90 %
$C_{12}H_{15}D_6N \cdot HCl \cdot 0.5H_2O$	Requires:	C 62.45, H 7.42, D 5.24, N 6.07 %, H_2O 3.90 %
$C_{12}H_{15}D_6N \cdot HCl$	Requires:	C 64.98, H 7.27, D 5.45, N 6.32 %

The elemental analyses fall somewhat outside those expected for anhydrous material; the presence of water is reasonably expected from the method of purification and/or the type of material, and the "best-fit" hydrated molecular formula is given. In the absence of a Karl-Fischer water analysis, we recommend that the "best-fit" water content be used when determining corrected purity.


The available quantity of custom-synthesised material is always small, and this limits the extent and type of analytical data which can be obtained. This Certificate is presented in descriptive format for use by analytical chemists who are trained in the use of custom-synthesised materials. Custom materials often contain higher levels of residual solvents and/or water, and we urge you to use the corrected purity where needed rather than the raw HPLC purity. This compound is intended for use as an analytical reference material and it is not for human administration. Structures are shown with relative stereochemistry unless otherwise specified.

The re-test date is assigned from experience gained with the material in the laboratory and/or on storage. It is not possible to perform formal storage studies because of the small amount of material available.




Proton NMR Spectrum of Memantine-d₆ HCl in DMSO-d₆

BDG SYNTHESIS




Lot Number: BDG 13810

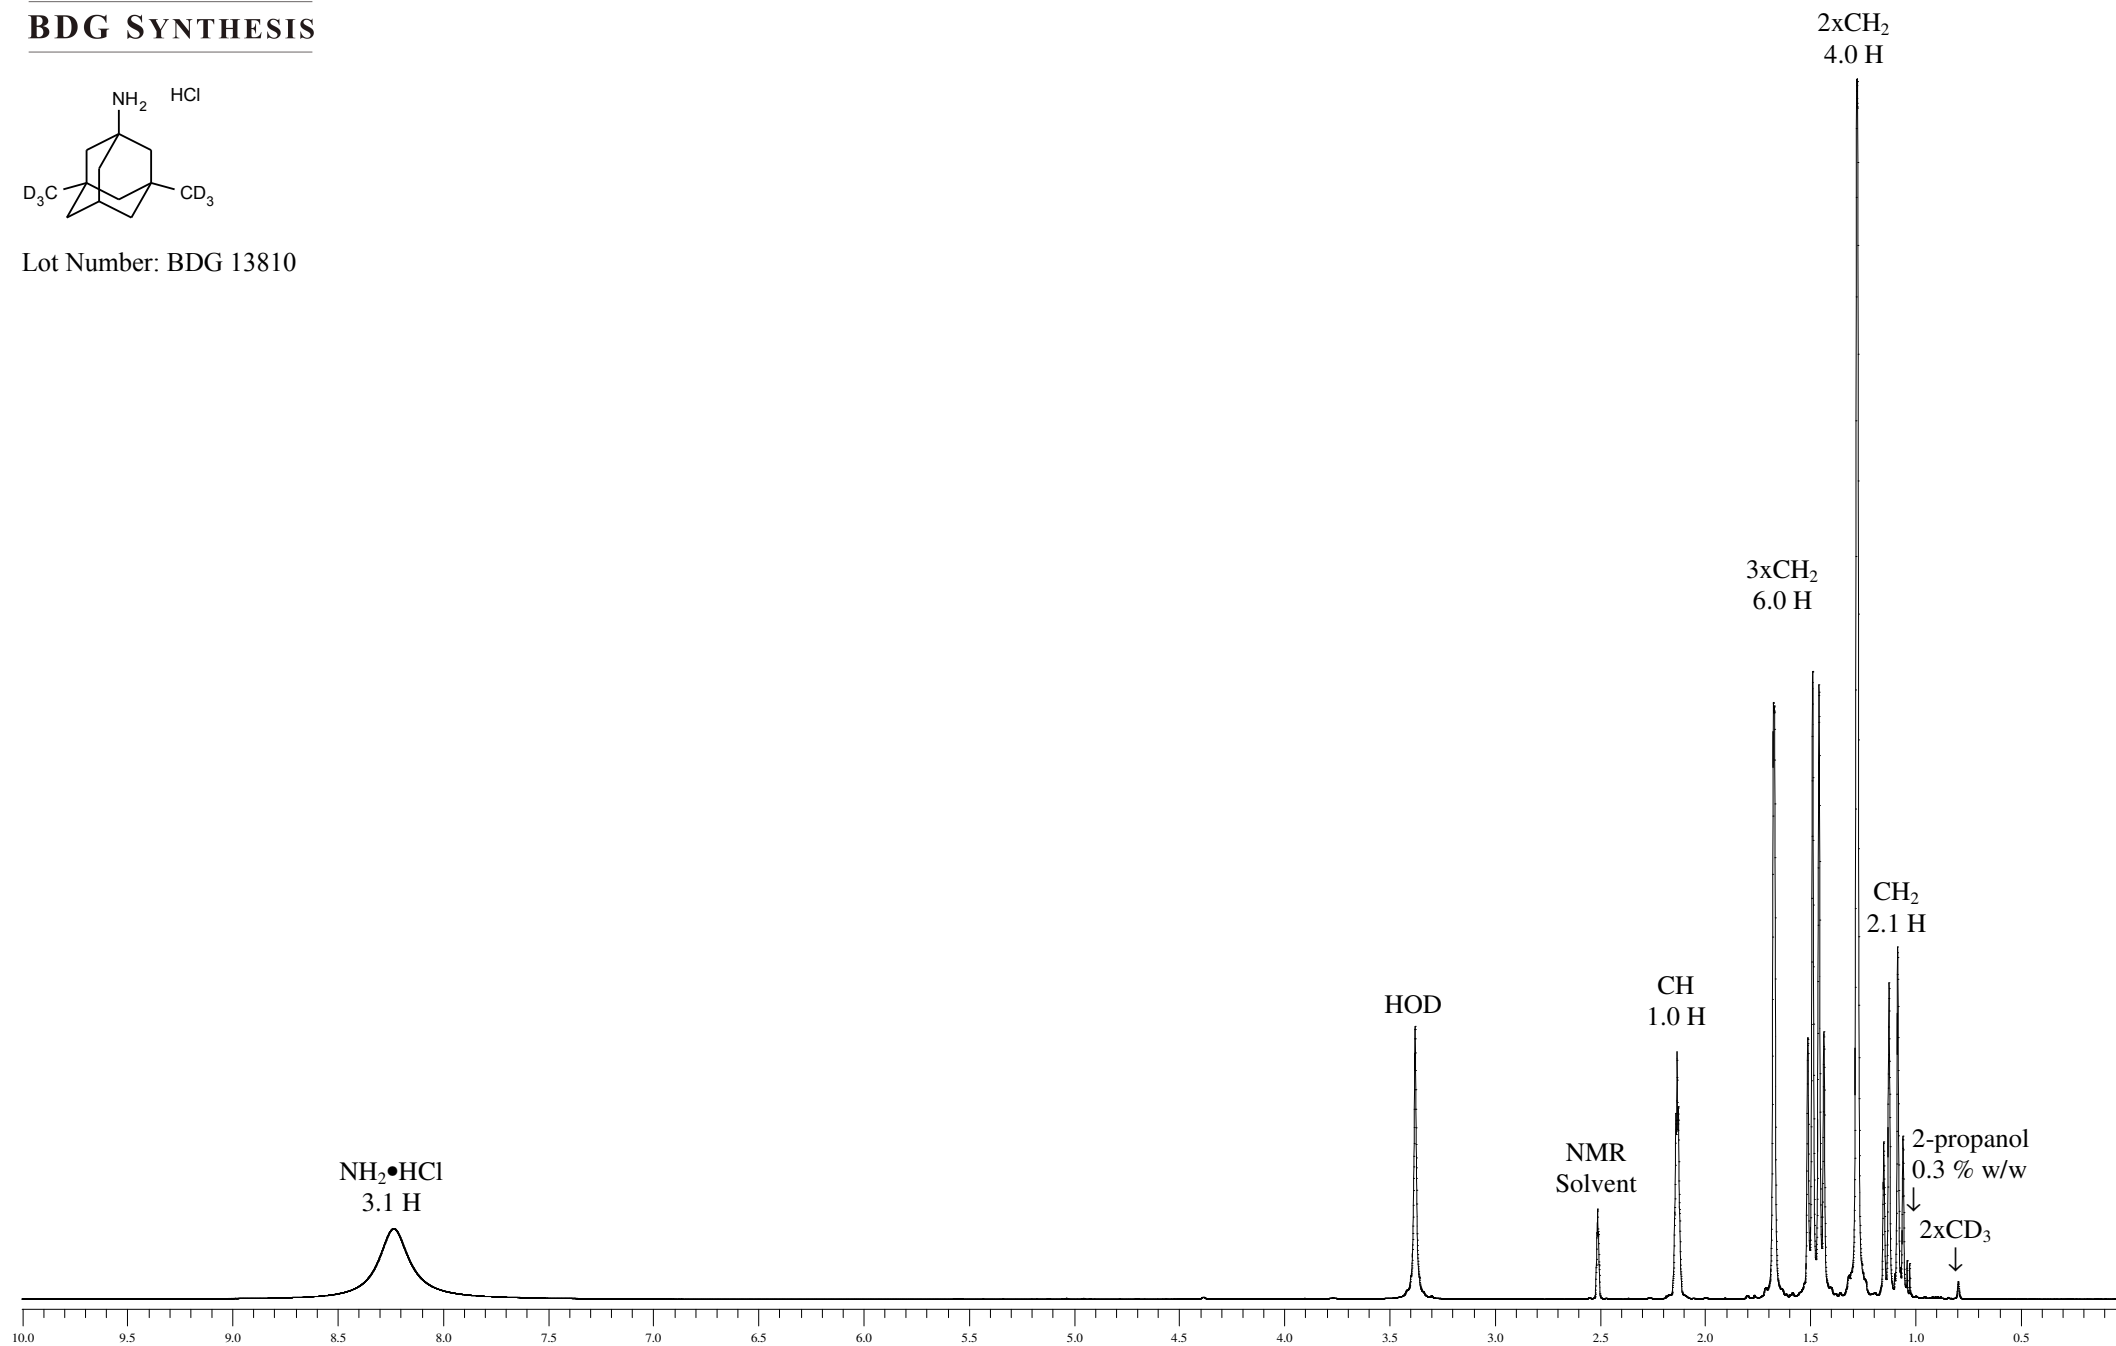




Carbon-13 NMR Spectrum of Memantine-d₆ HCl in DMSO-d₆

BDG SYNTHESIS




Lot Number: BDG 13810

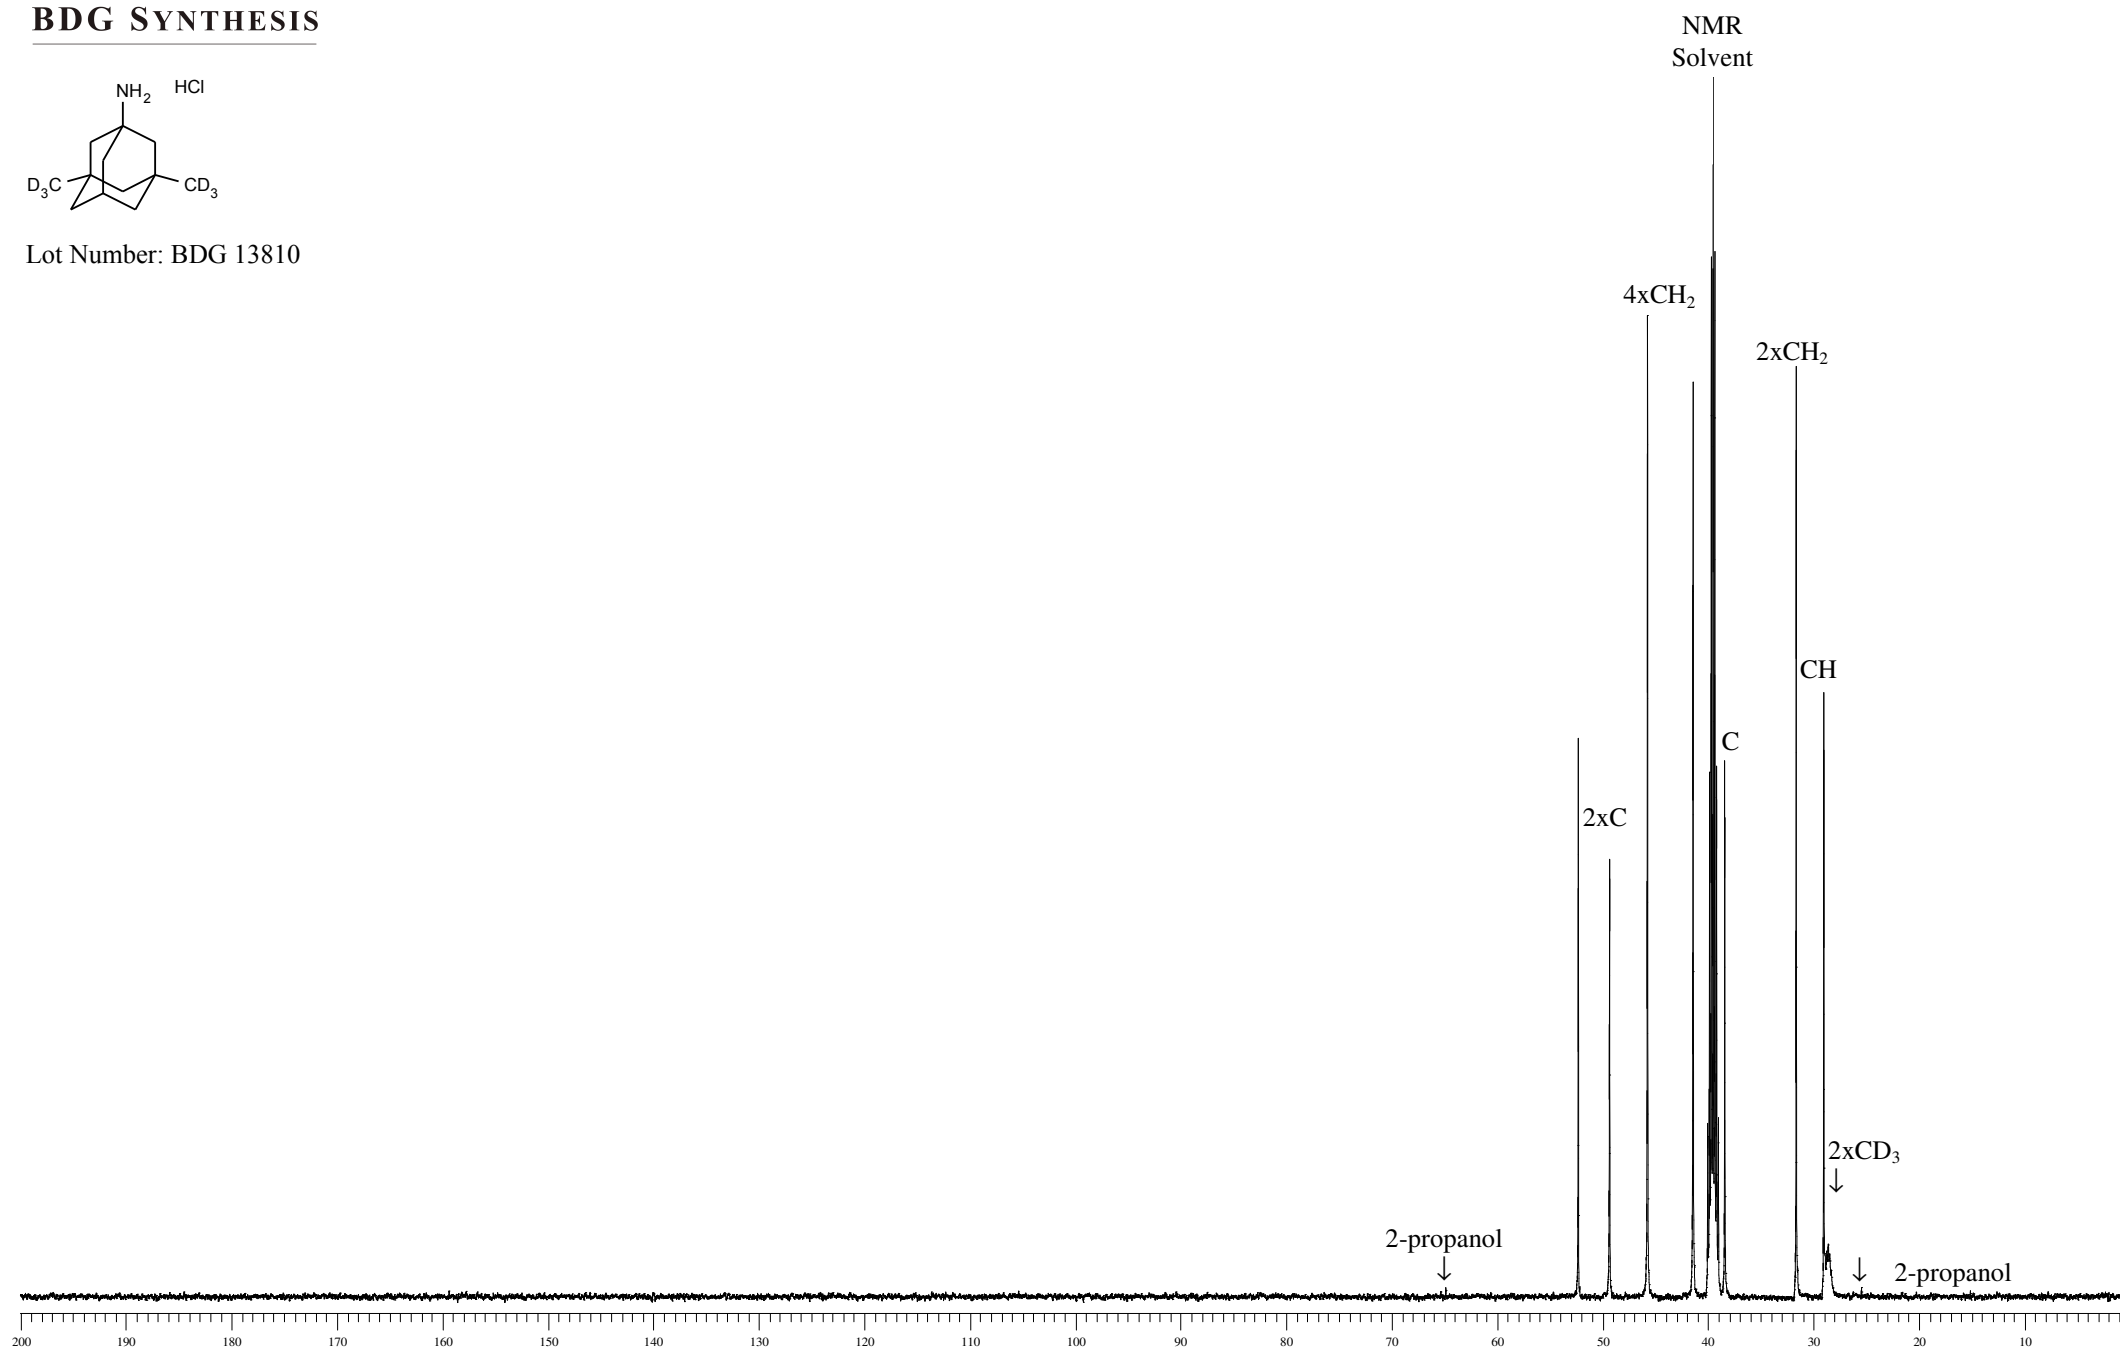

BDG - Analysis of Memantine-d6 HCl

Column : Phenomenex Luna C18(2) 5um 250 x 4.6 mm
 Guard : Phenomenex Security Guard C18 RP 4 x 3 mm
 Mobile Phase : 85:15 Water : Acetonitrile
 Flow Rate : 1.0 mL/min
 Sample Solvent : Initial Mobile Phase
 Column Temperature : 30C
 Injection Volume : 25 uL
 Detection : RI

Sample Name	BDG 13810	Instrument	AnalyticalLC01
Acquisition	23/07/2013, 19:43:38	Method (rev.)	LC10474a (13)
Sequence	BDG_23Jul2013d	Vial Position	1
Operator	solvation010\cerityadmin	Injection	2 of 2

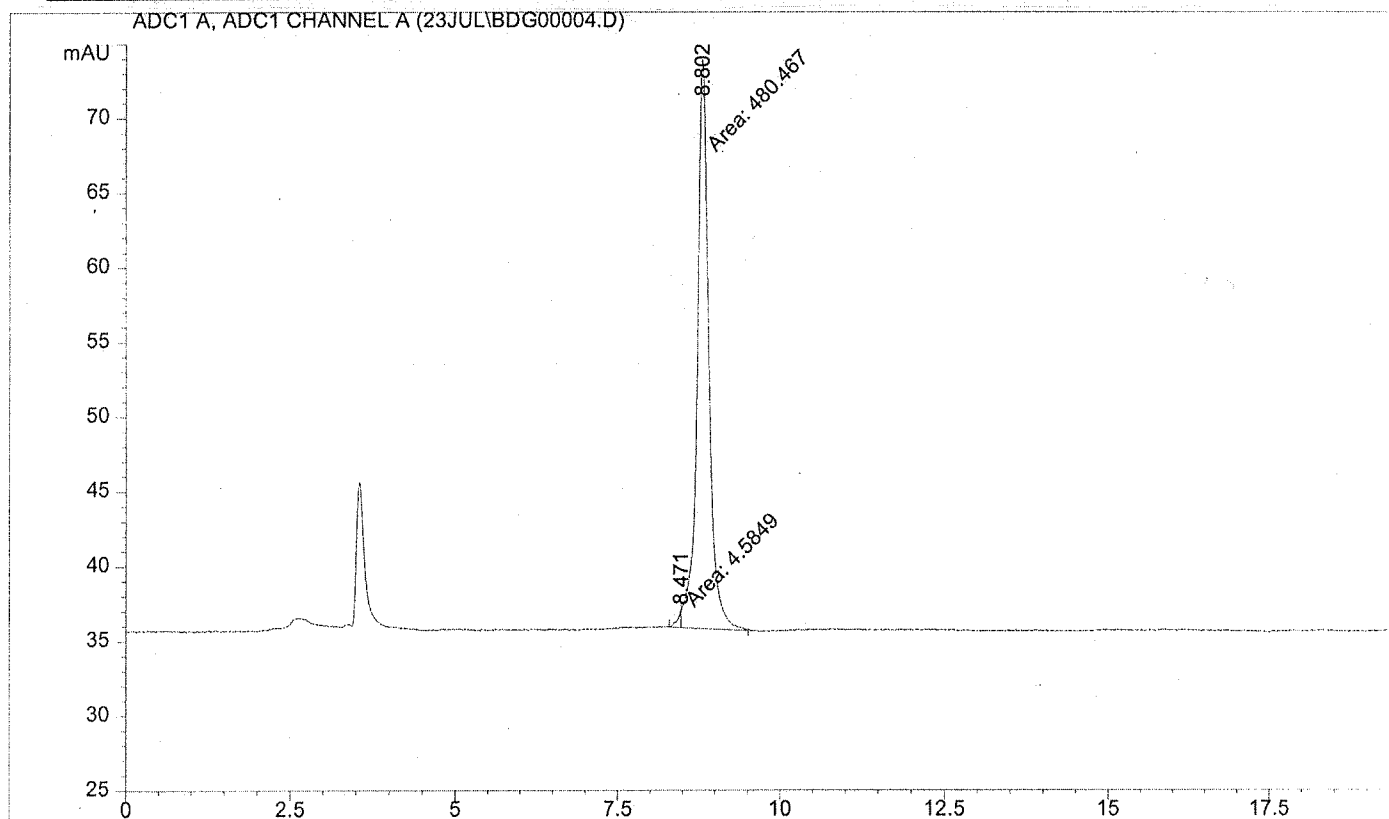

=====
 Area Percent Report
 =====

Sorted By : Signal
 Multiplier : 1.0000
 Dilution : 1.0000

Signal 1: ADC1 A, ADC1 CHANNEL A

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	8.471	MF	0.0674	4.58490	1.13317	0.9452
2	8.802	FM	0.2099	480.46664	38.15620	99.0548

Totals : 485.05154 39.28937

Results obtained with enhanced integrator!

=====
 *** End of Report ***