

Certificate of Analysis

BDG Synthesis certifies that this reference material meets or exceeds the specifications stated herein.

Barry Dent

Barry R. Dent, PhD, Director 9 September 2013

Name: Deshydroxyethylticagrelor-d₇

CAS Number: 220347-05-7 (unlabelled)

Structure:

Molecular Weight: $C_{21}H_{17}D_7F_2N_6O_3S = 485.56$

Lot Number: BDG 12845

Appearance: White, crystalline solid

Corrected Purity: 99.3 % (HPLC) - 0.2 % (ethanol) - 1.1 % (chloroform) - 0.4 % (heptane) = 97.6 %

Isotopic Purity: Under 0.5 % d₀

Re-test Date: 9 September 2018

Storage and Handling: Temperature: refrigerate for prolonged storage; may be handled and shipped at

ambient temperature.

Humidity: not believed to be hygroscopic; may be handled in normal laboratory

atmosphere.

Light: protect from strong sunlight.

Caution: only experienced laboratory personnel should handle the material.

Version 1 (1d606) 1/5

Phone: + 64 4 569 0520 Fax: + 64 4 569 0521 info@bdg.co.nz www.bdg.co.nz

Identity and Purity

Proton NMR Spectrum

Identity: The signals are consistent with the proposed structure and in accord with the literature where available. All signals are duplicated indicating two conformers of the product exist in solution.

Isotopic Labelling: signals at the sites of deuteration are absent, compared with the spectrum of unlabelled material, indicating clean deuteration.

Residual Solvents: small amounts of ethanol (0.2 % w/w) and heptane (0.4 % w/w) and chloroform (1.1 % w/w) are observed.

Impurities: no significant impurities are evident in the spectrum.

Carbon-13 NMR Spectrum

Identity: The signals are consistent with the proposed structure and in accord with the literature where available. All signals are duplicated indicating two conformers of the product exist in solution.

Isotopic Labelling: signals at the sites of deuteration have collapsed to small multiplets compared with the spectrum of unlabelled material, indicating clean deuteration.

High-resolution Mass Spectrum (ESI+)

Found m/z 486.2119. $C_{21}H_{18}D_7F_2N_6O_3S$ [M+H]⁺ requires m/z 486.2116. The deviation of 0.6 ppm is within normally accepted limits for the establishment of identity by HRMS. No signal for d_0 material was seen (detection limit about 0.5 %).

HPLC

A sharp, symmetrical peak is observed (99.3 %). Note: in the absence of reference materials for preparing calibration curves, it is assumed that all peaks have the same detector response. Where possible, the conditions of analysis follow a pharmacopeial or literature method, or have been adapted from same.

Elemental Analysis

Found: C 51.07, H 3.50, D 2.88, N 17.03 %

C₂₁H₁₇D₇F₂N₆O₃S·0.04CHCl₃ Requires: C 51.50, H 3.50, D 2.87, N 17.20 %, CHCl₃ 1.1%


C₂₁H₁₇D₇F₂N₆O₃S Requires: C 51.95, H 3.53, D 2.90, N 17.31 %

The elemental analyses fall within generally accepted limits for establishing the molecular formula given except the result for carbon. The results may also be taken to imply the absence of significant quantities of water or inorganic salts (which have not been elsewhere tested for because of sample size limitations).

The available quantity of custom-synthesised material is always small, and this limits the extent and type of analytical data which can be obtained. This Certificate is presented in descriptive format for use by analytical chemists who are trained in the use of custom-synthesised materials. Custom materials often contain higher levels of residual solvents and/or water, and we urge you to use the corrected purity where needed rather than the raw HPLC purity. This compound is intended for use as an analytical reference material and it is not for human administration. Structures are shown with relative stereochemistry unless otherwise specified.


The re-test date is assigned from experience gained with the material in the laboratory and/or on storage. It is not possible to perform formal storage studies because of the small amount of material available.



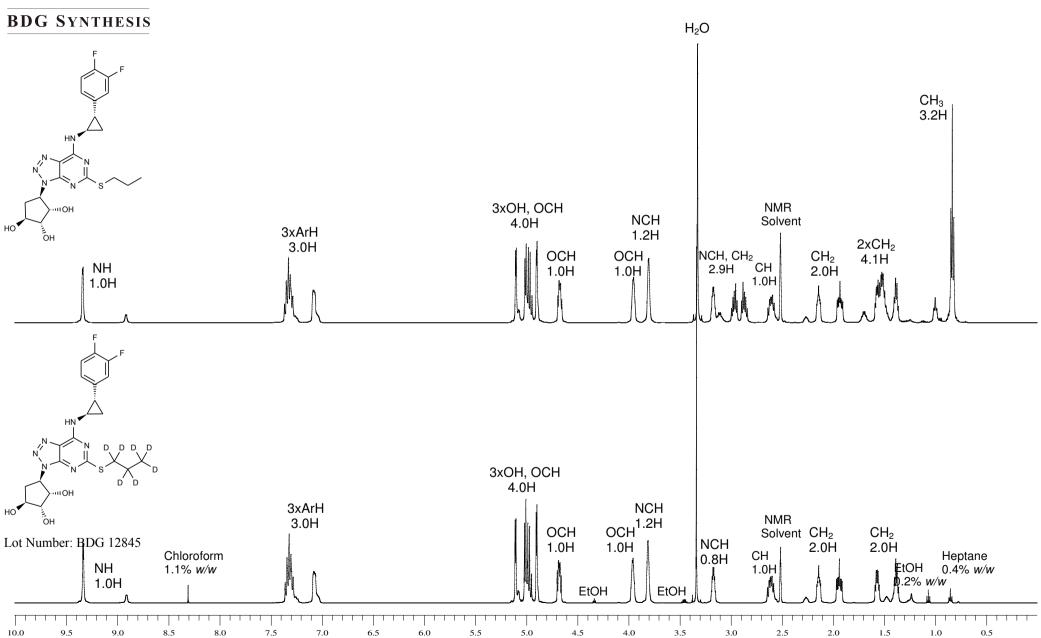





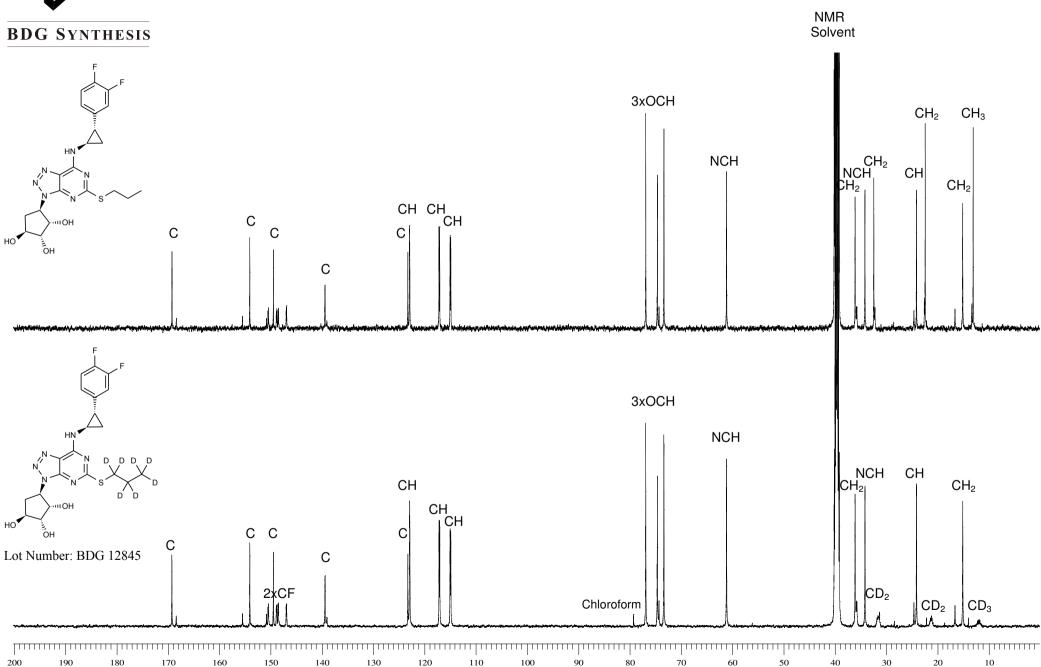

BDG - Analysis of Deshydroxyethylticagrelor-d7

Column: Phenomenex Luna C18(2) 5um 250 x 4.6 mm


Guard : Phenomenex Security Guard C18 RP 4 x 3 mm Mobile Phase : 50:50 20 mM Potassium diHydrogen Phosphate pH=3.0 : Acetonitrile

Flow Rate: 1.0 mL/min

Sample Solvent: 50:50 Water: Acetonitrile

Column Temperature : 20C Injection Volume : 10 uL Detection : UV at 300 nm

Sample Name	BDG 12845	Instrument	AnalyticalLC01
Acquisition	09/09/2013, 14:26:01	Method (rev.)	LC10585b (2)
Sequence	BDG_09Sep2013a	Vial Position	3
Operator	solvation010\cerityadmin	Injection	1 of 2

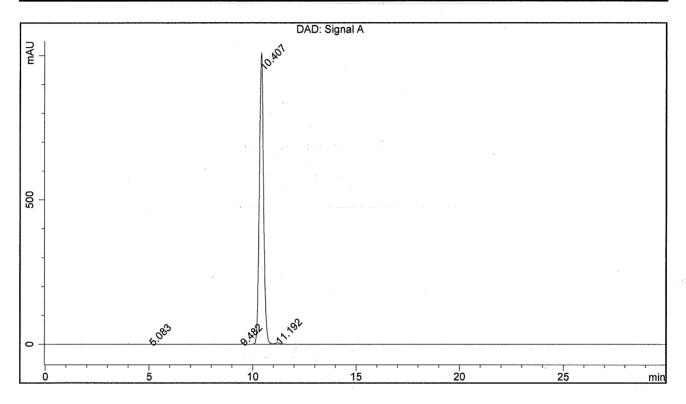

Area Percent Report

Peak#	RT	Peak Height	Peak Area	Width	Area %
1	5.08 min	0.6556	6.2712	0.1436 min	0.043 %
2	9.48 min	0.3713	5.4479	0.2192 min	0.037 %
3	10.41 min	1008.0308	14440.3507	0.2191 min	99.258 %
4	11.19 min	4.9800	96.1632	0.2853 min	0.661 %