

Certificate of Analysis

leil Beare

BDG Synthesis certifies that this reference material meets or exceeds the specifications stated herein.

Neil Beare, PhD, Director 1 December 2016

Name: N-Desethylbrinzolamide Oxalate

CAS Number: 404034-55-5 (free base)

Structure:

Molecular Weight: $C_{10}H_{17}N_3O_5S_3 \cdot C_2H_2O_4 = 445.49$

• Custom synthesis of analytical reference standards, metabolites, stable isotope labelled compounds

Lot Number: BDG 16811.1-0

Appearance: White, crystalline solid

Purity By HPLC: 100.0 % **Loss On Drying:** < 3.0 %

Re-test Date: 1 December 2017

Storage and Handling: Temperature: refrigerate for prolonged storage; may be handled and shipped at

ambient temperature.

Humidity: not believed to be hygroscopic; may be handled in normal laboratory

atmosphere.

Light: protect from strong sunlight.

Caution: only experienced laboratory personnel should handle the material.

Version 1 (1d955) 1/5

Wellington, New Zealand.

Phone: + 64 4 569 0520 Fax: + 64 4 569 0521

Identity and Purity

Proton NMR Spectrum

Identity: the signals are consistent with the proposed structure and in accord with literature where available.

Residual Solvents: a trace (under 0.1 % w/w) of methyl t-butyl ether is observed.

Impurities: no significant impurities are evident in the spectrum.

Carbon-13 NMR Spectrum

Identity: the signals are consistent with the proposed structure and in accord with literature where available.

High-resolution Mass Spectrum (TOF MS ES+)

Found m/z 356.0406. $C_{10}H_{18}N_3O_5S_3$ [M+H]⁺ requires m/z 356.0409. The deviation of 0.8 ppm is within normally accepted limits for the establishment of identity by HRMS.

HPLC

A sharp, symmetrical peak is observed (100.0 %). The minor peak at 3 minutes has been confirmed as Oxalic Acid by spiking experiments. Note: in the absence of reference materials for preparing calibration curves, it is assumed that all peaks have the same detector response. Where possible, the conditions of analysis follow a pharmacopeial or literature method, or have been adapted from same.

Elemental Analysis

 $C_{10}H_{17}N_3O_5S_3\cdot C_2H_2O_4$


Found: C 32.40, H 4.22, N 9.41 % Requires: C 32.35, H 4.30, N 9.43 %

The elemental analyses fall within generally accepted limits for establishing the molecular formula given. The results may also be taken to imply the absence of significant quantities of water or inorganic salts (which have not been elsewhere tested for because of sample size limitations).


The available quantity of custom-synthesised material is always small, and this limits the extent and type of analytical data which can be obtained. This Certificate is presented in descriptive format for use by analytical chemists who are trained in the use of custom-synthesised materials. Custom materials often contain higher levels of residual solvents and/or water, and we urge you to use the corrected purity where needed rather than the raw HPLC purity. This compound is intended for use as an analytical reference material and it is not for human administration. Structures are shown with relative stereochemistry unless otherwise specified.

The re-test date is assigned from experience gained with the material in the laboratory and/or on storage. It is not possible to perform formal storage studies because of the small amount of material available.

BDG SYNTHESIS




Lot Number: BDG 16811.1

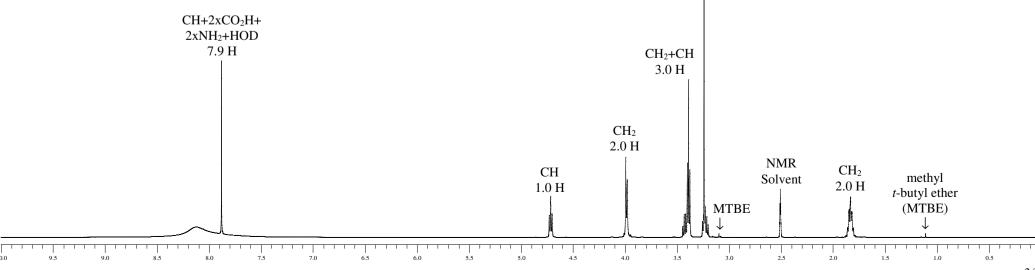

OCH₃+CH 4.0 H



BDG SYNTHESIS

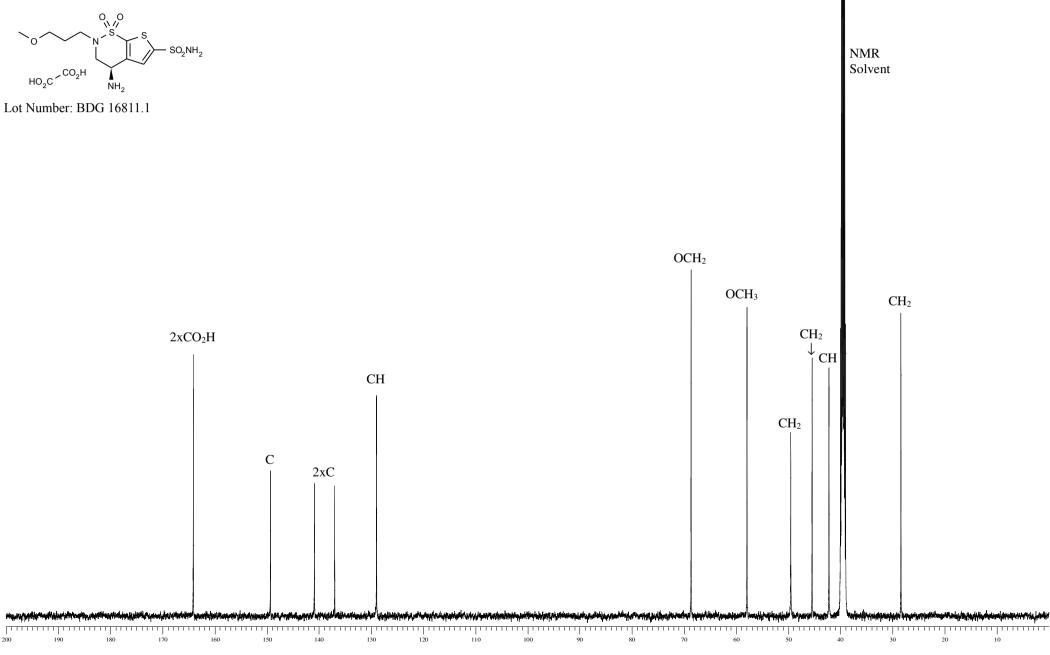

BDG - Analysis of AL-8520A

Column : Phenomenex Luna C18 5um 250 x 4.6 mm Guard : Phenomenex Security Guard C18 4 x 3 mm

Mobile Phase A: 90:10 10 mM Potassium diHydrogen Phosphate pH = 2.5: Methanol

Mobile Phase B: 50:50 Water: Acetonitrile


Gradient (A:B): T0=100:0, T20=0:100, T24=0:100, T25=100:0, T30=100:0

Flow Rate: 1.0 mL/min

Sample Solvent : Initial Mobile Phase

Column Temperature : 20 C Injection Volume : 10 uL Detection : UV at 250 nm

Sample Name	BDG 16811.1	Instrument	AnalyticalLC01
Acquisition	01/12/2016, 19:40:40	Method (rev.)	LC10250c (19)
Sequence	BDG_01Dec2016c	Vial Position	1
Operator	solvation010\cerityadmin	Injection	1 of 1

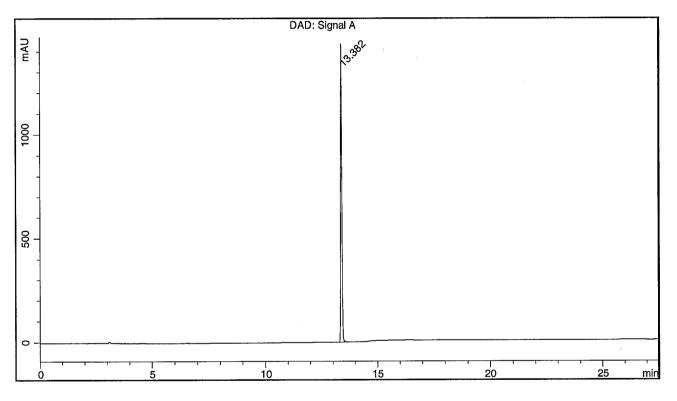

Area Percent Report

Peak#	RT	Peak Height	Peak Area	Width	Area %
1	13.38 min	1441.9545	5458.3886	0.0602 min	100.000 %