

BDG SYNTHESIS

Certificate of Analysis


BDG Synthesis certifies that this reference material meets or exceeds the specifications stated herein.

Barry Dent

Barry R. Dent, PhD, Director
6 September 2009

Name: Harman-d₄
CAS Number: 486-84-0 (unlabelled)

Structure:



Molecular Weight: C₁₂H₆D₄N₂ = 186.25
Lot Number: BDG 5849.3
Appearance: Pale, tan, crystalline powder
Purity By HPLC: 99.9 %
Isotopic Purity: Under 0.5 % d₀
Re-test Date: 6 September 2014
Storage and Handling: Temperature: ambient laboratory temperature; may be refrigerated.
Humidity: not believed to be hygroscopic; may be handled in normal laboratory atmosphere.
Light: protect from strong sunlight.
Caution: only experienced laboratory personnel should handle the material.

Identity and Purity

Proton NMR Spectrum

Identity: the signals are consistent with the proposed structure and in accord with literature where available.

Isotopic Labelling: signals at the sites of deuteration are greatly diminished, compared with the spectrum of unlabelled material, indicating clean deuteration.

Residual Solvents: no residual solvents are observed.

Impurities: no significant impurities are evident in the spectrum.

Carbon-13 NMR Spectrum

Identity: the signals are consistent with the proposed structure and in accord with literature where available.

Isotopic Labelling: signals at the sites of deuteration have collapsed to small multiplets compared with the spectrum of unlabelled material, indicating clean deuteration. One of the labelled signals appears absent as it coincides with another that arises from a quaternary carbon.

High-resolution Mass Spectrum (ESI-)

Found m/z 185.1026. $C_{12}H_3D_4N_2$ [M-H]⁻ requires m/z 185.1022. The deviation of 2.2 ppm is within normally accepted limits for the establishment of identity by HRMS. No signal for d_0 material was seen (detection limit about 0.5 %).

HPLC

A sharp, symmetrical peak is observed (99.9 %). Note: in the absence of reference materials for preparing calibration curves, it is assumed that all peaks have the same detector response. Where possible, the conditions of analysis follow a pharmacopeial or literature method, or have been adapted from same.

Elemental Analysis

	Found:	C 77.11, H 3.18, D 4.24, N 15.14 %
$C_{12}H_6D_4N_2$	Requires:	C 77.39, H 3.25, D 4.33, N 15.04 %

The elemental analyses fall within generally accepted limits for establishing the molecular formula given. The results may also be taken to imply the absence of significant quantities of water or inorganic salts (which have not been elsewhere tested for because of sample size limitations).




The available quantity of custom-synthesised material is always small, and this limits the extent and type of analytical data which can be obtained. This Certificate is presented in descriptive format for use by analytical chemists who are trained in the use of custom-synthesised materials. Custom materials often contain higher levels of residual solvents and/or water, and we urge you to use the corrected purity where needed rather than the raw HPLC purity. This compound is intended for use as an analytical reference material and it is not for human administration. Structures are shown with relative stereochemistry unless otherwise specified.

The re-test date is assigned from experience gained with the material in the laboratory and/or on storage. It is not possible to perform formal storage studies because of the small amount of material available.




Proton NMR Spectrum of Harman (top) and Harman-d₄ (bottom) in Methanol-d₄

BDG SYNTHESIS

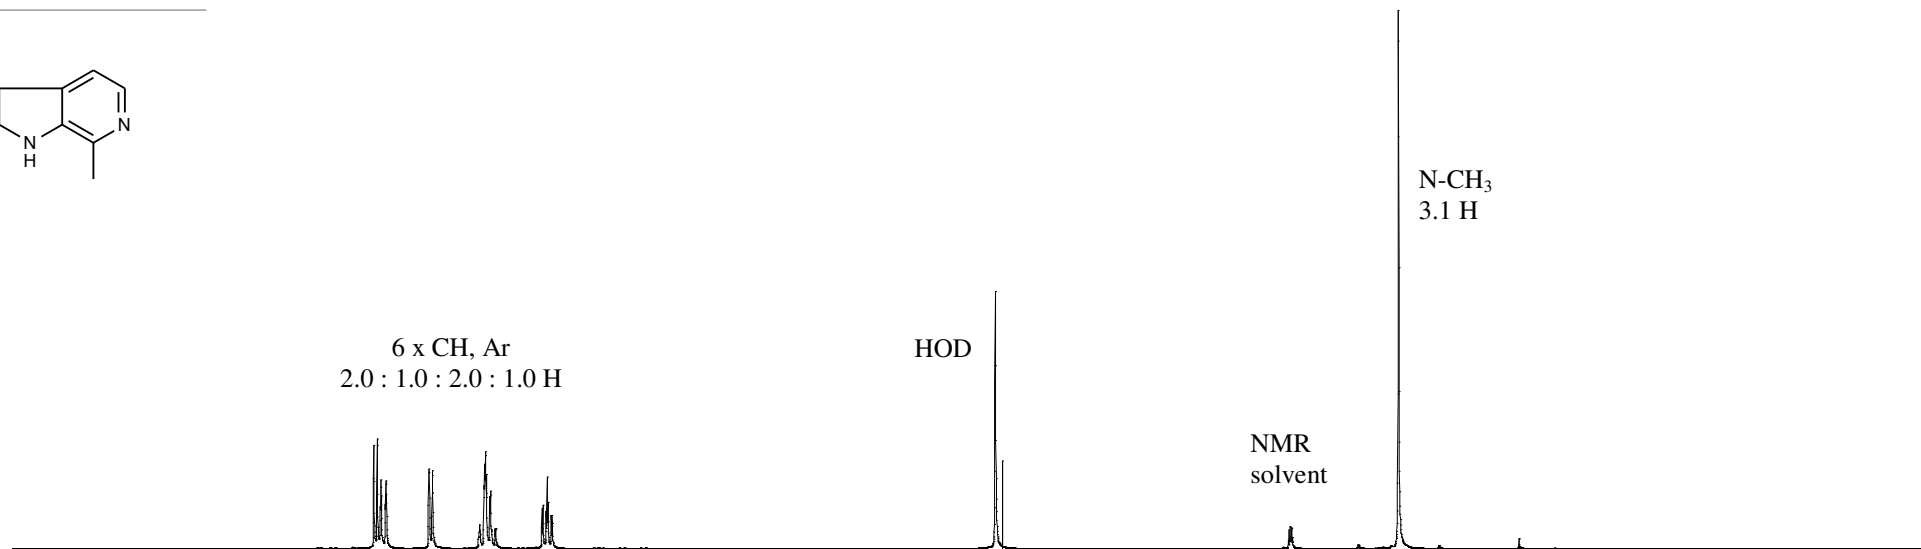




Lot Number: BDG 5849.3

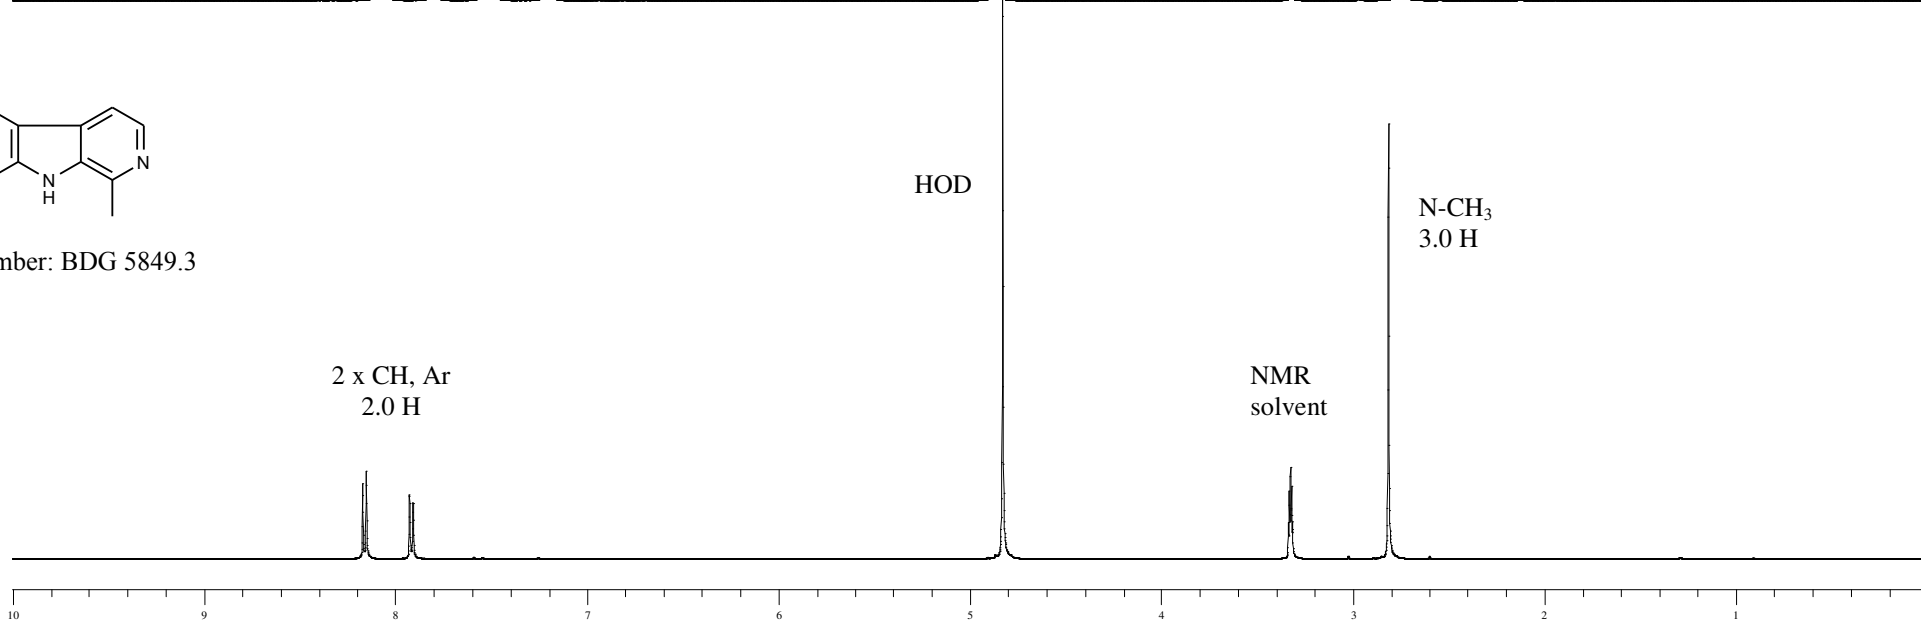




Carbon-13 NMR Spectrum of Harman (top) and Harman-d₄ (bottom) in Methanol-d₄

BDG SYNTHESIS

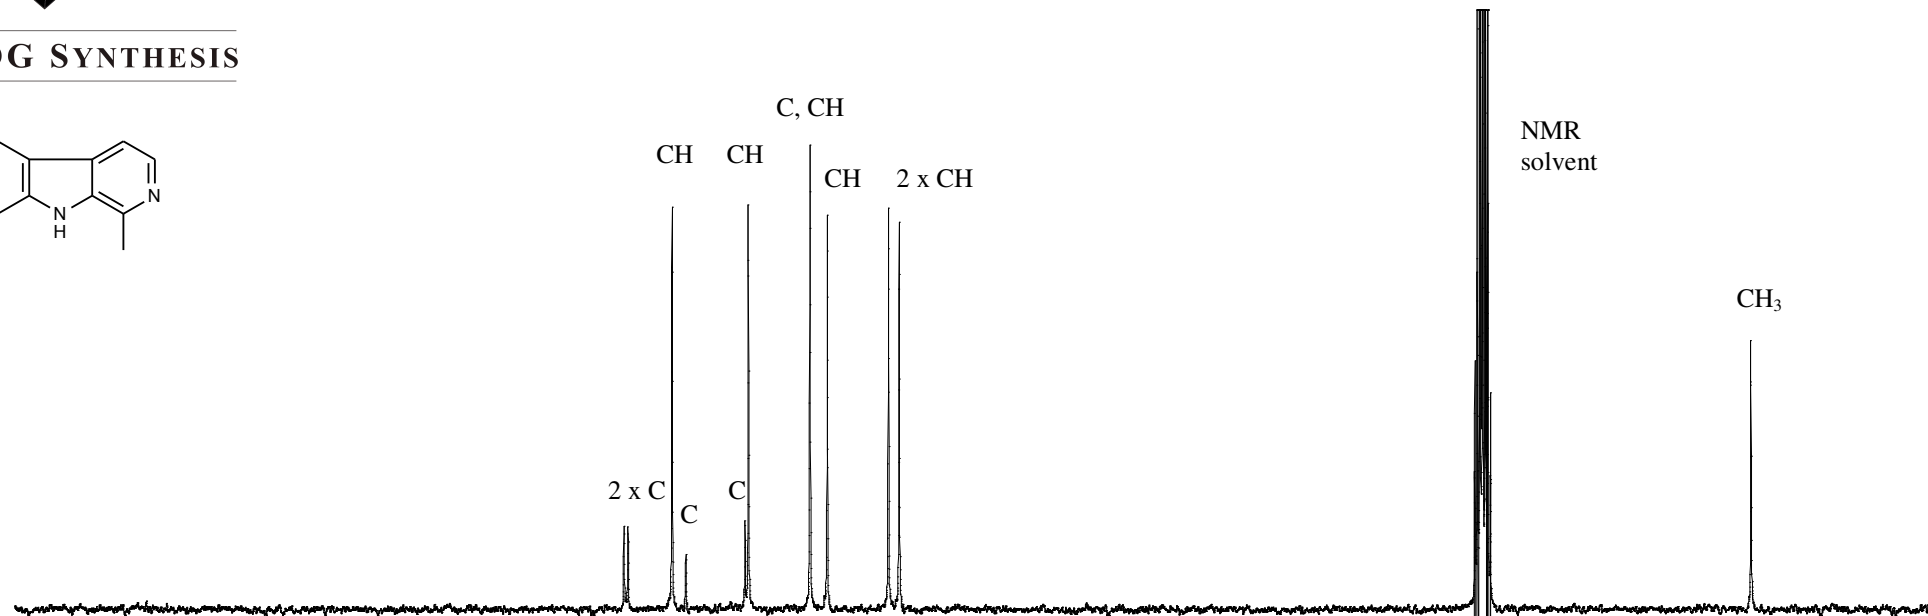


Lot Number: BDG 5849.3

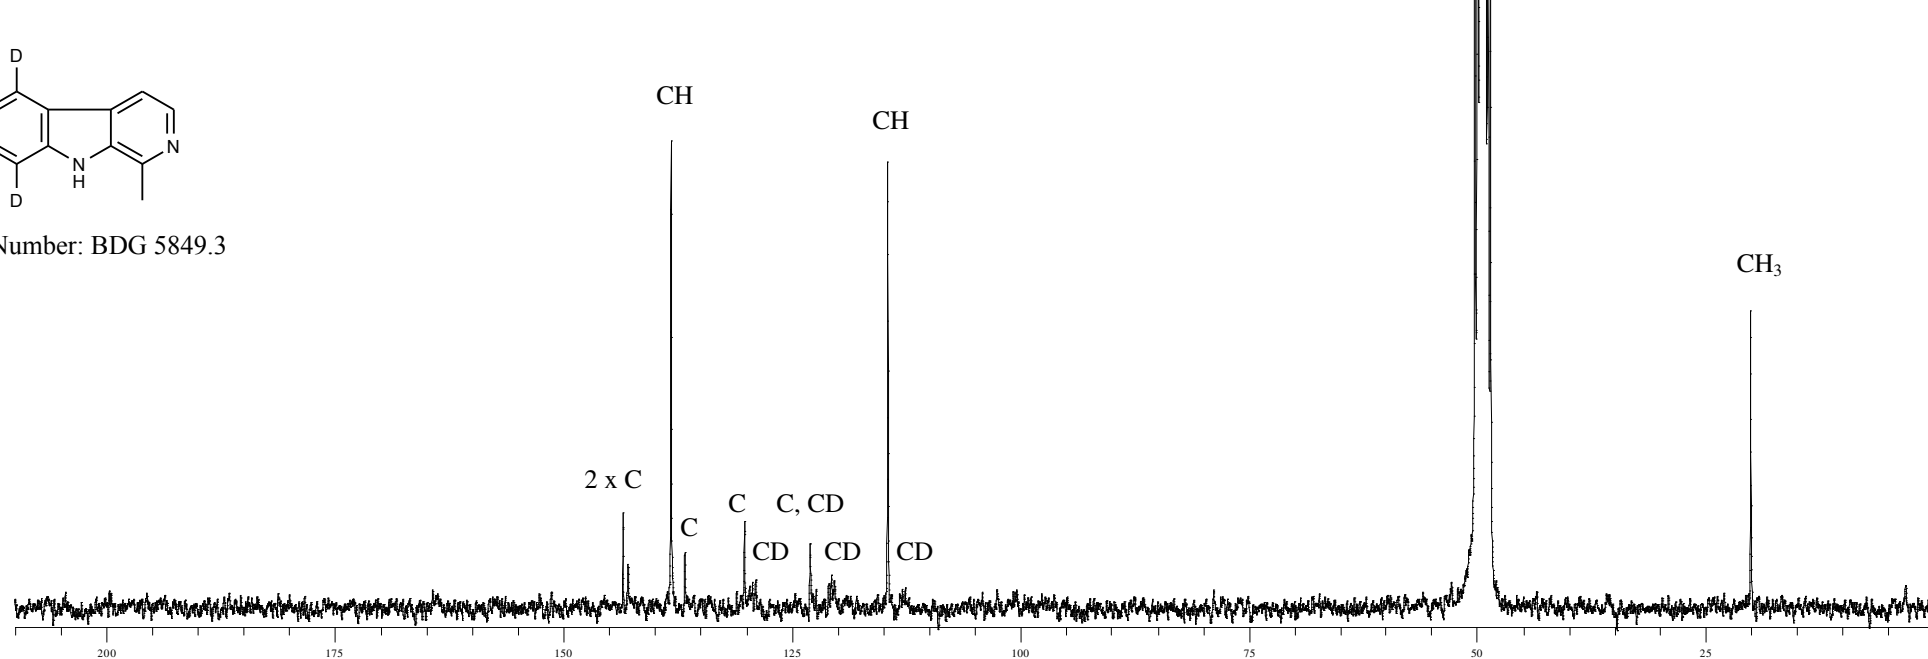

BDG - Analysis of Harman-d4

Column : Phenomenex Luna C18(2) 5um 250 x 4.6 mm
 Guard : Phenomenex Security Guard C18 RP 4 x 3 mm
 Mobile Phase A: Water + 0.1% Trifluoroacetic Acid
 Mobile Phase B: Acetonitrile + 0.1% Trifluoroacetic Acid
 Gradient (A:B) : T0=80:20, T20=50:50, T24=50:50, T27=80:20, T30=80:20
 Flow Rate : 1.0 mL/min
 Sample Solvent : 4:1 Water : Acetonitrile
 Injection Volume : 10 uL
 Column Temperature : 20C
 Detection : UV at 240 nm

Sample Name	BDG 5849.3	Instrument	AnalyticalLC01
Acquisition	06/09/2009, 17:18:44	Method (rev.)	LC10337a (9)
Sequence	BDG_06Sep2009f - Reprocessed	Vial Position	2
Operator	solvation010\cerityadmin	Injection	2 of 2

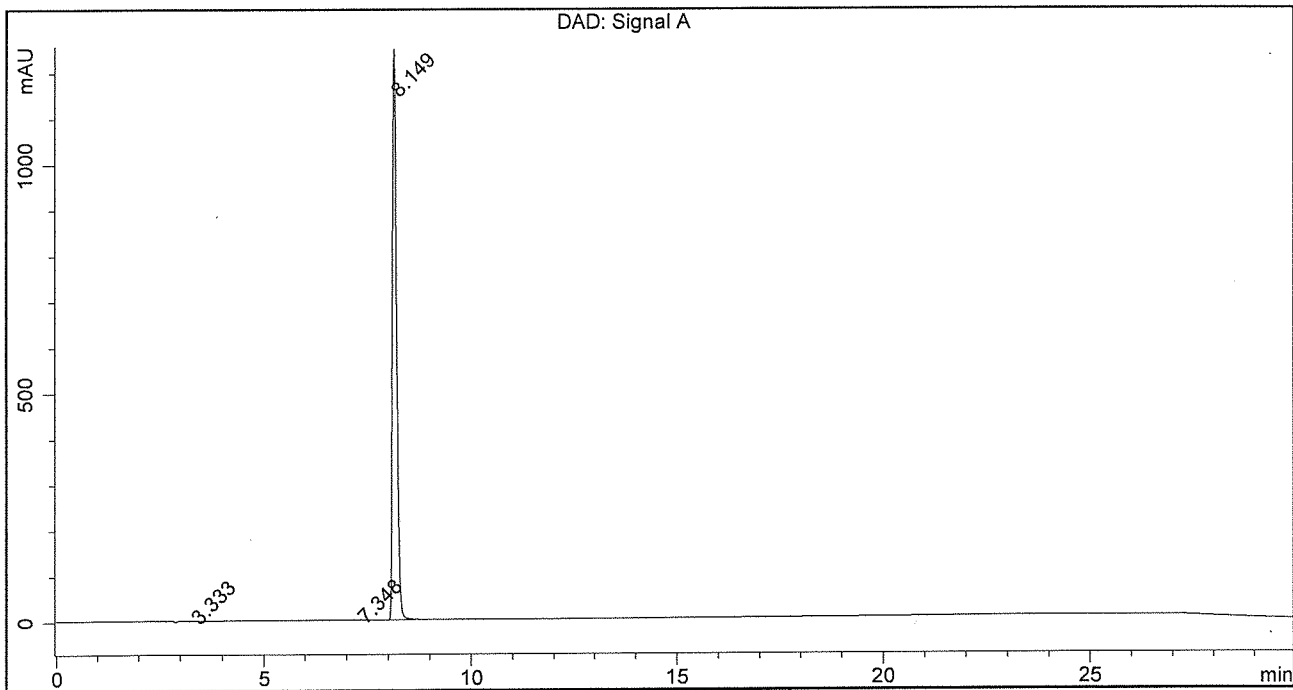

Area Percent Report

Peak#	RT	Peak Height	Peak Area	Width	Area %
1	3.33 min	0.3324	2.5265	0.1087 min	0.029 %
2	7.35 min	0.4279	2.7584	0.1012 min	0.031 %
3	8.15 min	1249.6171	8837.7082	0.1105 min	99.940 %