

Certificate of Analysis

BDG Synthesis certifies that this reference material meets or exceeds the specifications stated herein.

Barry Dent

Barry R. Dent, PhD, Director 23 November 2009

Name: RS-94287

CAS Number: 5294-61-1

Structure:

Molecular Weight: $C_{14}H_{21}N_3O = 247.34$

Lot Number: BDG 8948

Appearance: Off-white, crystalline solid

Corrected Purity: 99.9 % (HPLC) - 0.8 % (ethyl acetate) = 99.1 %

Re-test Date: 23 November 2010

Storage and Handling: Temperature: ambient laboratory temperature; may be refrigerated.

Humidity: not believed to be hygroscopic; may be handled in normal laboratory

atmosphere.

Light: protect from strong sunlight.

Caution: only experienced laboratory personnel should handle the material.

Version 1 (*Id72*) 1/5

• Custom synthesis of analytical reference standards, metabolites, stable isotope labelled compounds

• Contract research • BDG Synthesis is a division of B Dent Global Limited

Phone: + 64 4 569 0520 info@bdg.co.nz

Fax:

+6445690521

info@bdg.co.nz www.bdg.co.nz

Identity and Purity

Proton NMR Spectrum

Identity: the signals are consistent with the proposed structure and in accord with literature where available.

Residual Solvents: a small amount of ethyl acetate (0.8 % w/w) is observed.

Impurities: no significant impurities are evident in the spectrum.

Carbon-13 NMR Spectrum

Identity: the signals are consistent with the proposed structure and in accord with literature where available.

High-resolution Mass Spectrum (ESI+)

Found m/z 248.1753. $C_{14}H_{22}N_3O$ [M+H]⁺ requires m/z 248.1757. The deviation of 2.7 ppm is within normally accepted limits for the establishment of identity by HRMS.

HPLC

A sharp, symmetrical peak is observed (99.9 %). Note: in the absence of reference materials for preparing calibration curves, it is assumed that all peaks have the same detector response. Where possible, the conditions of analysis follow a pharmacopeial or literature method, or have been adapted from same.

Elemental Analysis

Found: C 67.90, H 8.84, N 17.21 %


C₁₄H₂₁N₃O Requires: C 67.98, H 8.56, N 16.99 %

The elemental analyses fall within generally accepted limits for establishing the molecular formula given. The results may also be taken to imply the absence of significant quantities of water or inorganic salts (which have not been elsewhere tested for because of sample size limitations).


The available quantity of custom-synthesised material is always small, and this limits the extent and type of analytical data which can be obtained. This Certificate is presented in descriptive format for use by analytical chemists who are trained in the use of custom-synthesised materials. Custom materials often contain higher levels of residual solvents and/or water, and we urge you to use the corrected purity where needed rather than the raw HPLC purity. This compound is intended for use as an analytical reference material and it is not for human administration. Structures are shown with relative stereochemistry unless otherwise specified.

The re-test date is assigned from experience gained with the material in the laboratory and/or on storage. It is not possible to perform formal storage studies because of the small amount of material available.






Lot Number: BDG 8948

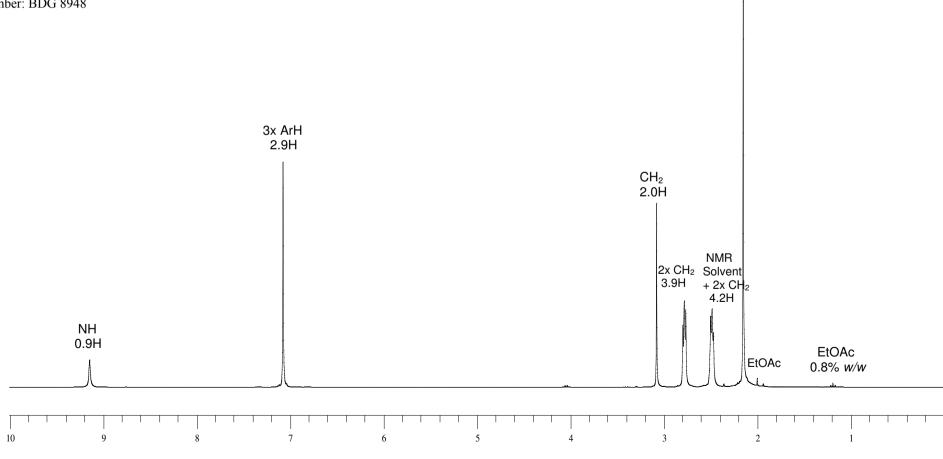


2x CH₃, NH 6.5H







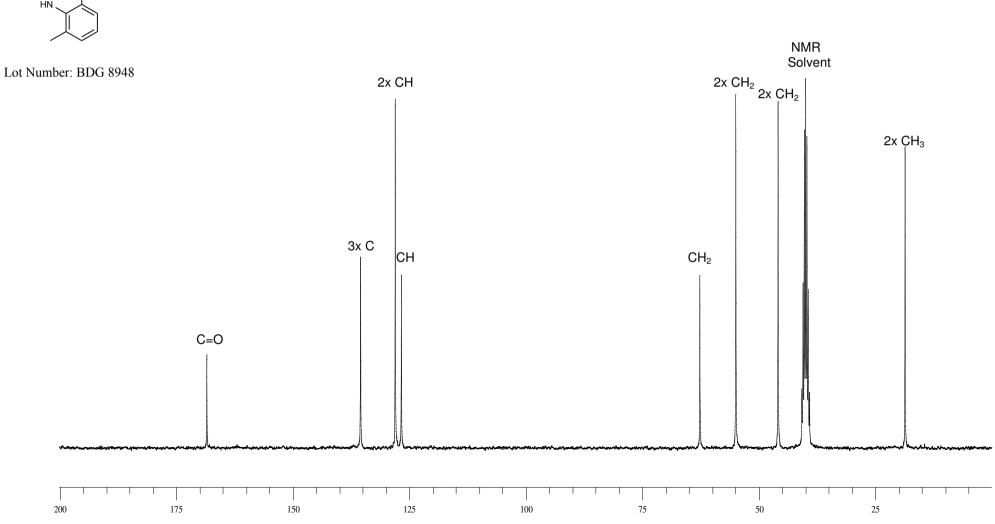

BDG - Analysis of RS-94287

Column : Phenomenex Luna C18(2) 5um 250 x 4.6 mm Guard : Phenomenex Security Guard C18 RP 4 x 3 mm

Mobile Phase A: 25 mM Potassium diHydrogen Phosphate pH=3.0

Mobile Phase B : Acetonitrile


Gradient (A:B): T0=90:10, T20=40:60, T24=40:60, T27=90:10, T30=90:10

Flow Rate : 1.0 mL/min

Sample Solvent: 4:1 Water: Acetonitrile

Column Temperature : 20C Injection Volume : 10 uL Detection : UV 225 nm

Sample Name	BDG 8948	Instrument	AnalyticalLC01
Acquisition	23/11/2009, 14:42:31 Method (rev.)		LC10354a (7)
Sequence	BDG_23Nov2009a	Vial Position	1
Operator	solvation010\cerityadmin	Injection	1 of 1

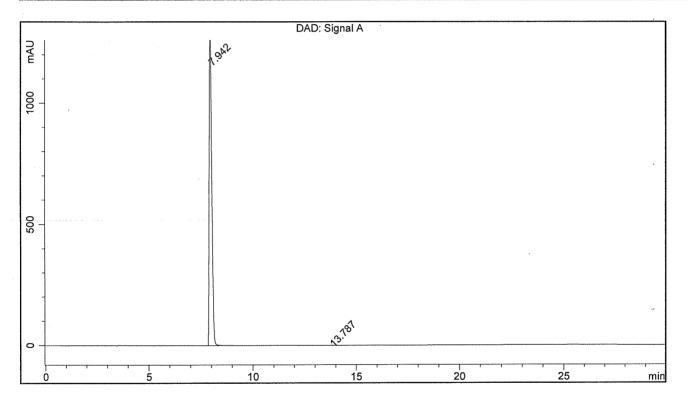

Area Percent Report

Peak#	RT	Peak Height	Peak Area	Width	Area %.
1	7.94 min	1306.8825	11296.3869	0.1368 min	99.971 %
2	13.79 min	0.5209	3.2787	0.0954 min	0.029 %