

Certificate of Analysis

BDG Synthesis certifies that this reference material meets or exceeds the specifications stated herein.

Barry Dent

Barry R. Dent, PhD, Director 21 March 2011

Name: 1-(5-Hydroxy-2-pyrimidinyl)piperazine Bis(trifluoroacetate)

CAS Number: 55745-85-2 (free base)

Structure:

2 CF₃COOH

Molecular Weight: $C_8H_{12}N_4O \cdot 2C_2HF_3O_2 = 408.25$

Lot Number: BDG 9122.1-04

Appearance: White, crystalline solid

Corrected Purity: 99.9 % (HPLC) - 0.3 % (water) = 99.6 %

Re-test Date: 21 March 2012

Storage and Handling: Temperature: refrigerate for prolonged storage; may be handled and shipped at

ambient temperature.

Humidity: not believed to be hygroscopic; may be handled in normal laboratory

atmosphere.

Light: protect from strong sunlight.

Caution: only experienced laboratory personnel should handle the material.

Identity and Purity

Proton NMR Spectrum

Identity: the signals are consistent with the proposed structure and in accord with literature where available. Residual Solvents: no residual solvents are observed.

Impurities: no significant impurities are evident in the spectrum.

Carbon-13 NMR Spectrum

Identity: the signals are consistent with the proposed structure and in accord with literature where available.

High-resolution Mass Spectrum (ESI+)

Found m/z 181.1088. $C_8H_{13}N_4O$ [M+H]⁺ requires m/z 181.1084. The deviation of 2.2 ppm is within normally accepted limits for the establishment of identity by HRMS.

HPLC

A sharp, symmetrical peak is observed (99.9 %). Note: in the absence of reference materials for preparing calibration curves, it is assumed that all peaks have the same detector response. Where possible, the conditions of analysis follow a pharmacopeial or literature method, or have been adapted from same.

Elemental Analysis

Found: C 36.04, H 3.94, F 28.70, N 14.13 % C₈H₁₂N₄O·2C₂HF₃O₂·0.1H₂O Requires: C 35.15, H 3.49, F 27.80, N 13.66 % Requires: C 35.30, H 3.46, F 27.92, N 13.72 %

The elemental analyses fall slightly outside those expected for anhydrous material; the presence of water is reasonably expected from the method of purification and/or the type of material, and the "best-fit" hydrated molecular formula is given.

Karl-Fischer Analysis

Found: $H_2O 0.3 \%$ $C_8H_{12}N_4O \cdot 2C_2HF_3O_2 \cdot 0.1H_2O$ Requires: $H_2O 0.4 \%$

Of necessity, only a small sample could be used and only a single or duplicate analysis performed. We are unable to state what the errors in the reported water content are, but recommend that the result be used, as the best available, when determining corrected purity.

The available quantity of custom-synthesised material is always small, and this limits the extent and type of analytical data which can be obtained. This Certificate is presented in descriptive format for use by analytical chemists who are trained in the use of custom-synthesised materials. Custom materials often contain higher levels of residual solvents and/or water, and we urge you to use the corrected purity where needed rather than the raw HPLC purity. This compound is intended for use as an analytical reference material and it is not for human administration. Structures are shown with relative stereochemistry unless otherwise specified.

The re-test date is assigned from experience gained with the material in the laboratory and/or on storage. It is not possible to perform formal storage studies because of the small amount of material available.


BDG SYNTHESIS

$$N \longrightarrow OH$$

2 CF₃COOH


2xCH 1.8 H


Lot Number: BDG 9122.1

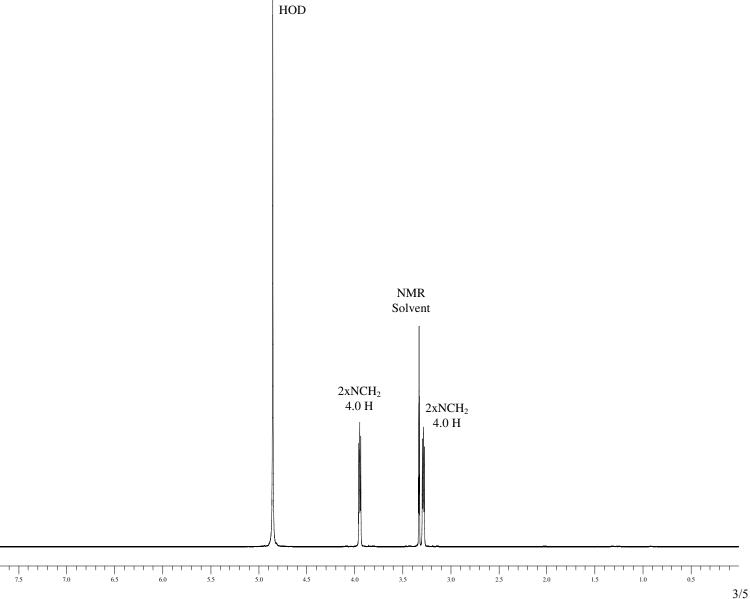

NMR Solvent





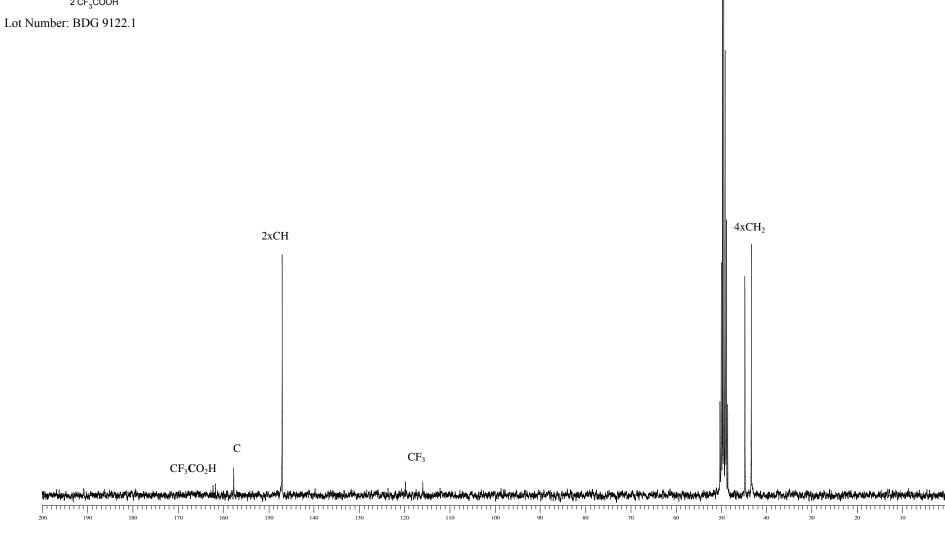

BDG - Analysis of 1-(5-Hydroxy-2-pyrimidinyl)piperazine Bis(trifluoroacetate)


Column : Phenomenex Luna C18(2) 5um 250 x 4.6 mm Guard : Phenomenex Security Guard C18 RP 4 x 3 mm

Mobile Phase A: 95:5 50mM Potassium diHydrogen Phosphate pH 3.0 : Acetonitrile Mobile Phase B: 70:30 50mM Potassium diHydrogen Phosphate pH 3.0 : Acetonitrile

Gradient (A:B): T0=100:0, T10=100:0, T25=0:100, T27=100:0, T30=100:0

Flow Rate: 1.0 mL/min Sample Solvent: Water Injection Volume: 10 uL Column Temperature: 20C Detection: UV at 240 nm

Sample Name	BDG 9122.1	Instrument	AnalyticalLC01
Acquisition	21/03/2011, 14:32:43	Method (rev.)	LC10327b (5)
Sequence	BDG_21Mar2011b - Reprocessed	Vial Position	1
Operator	solvation010\cerityadmin	Injection	1 of 1

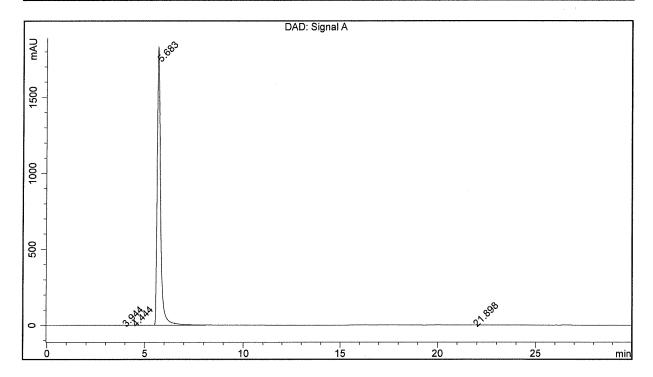

Area Percent Report

Peak#	RT	Peak Height	Peak Area	Width	Area %
1	3.94 min	0.5632	3.0645	0.0755 min	0.014 %
2	4.44 min	0.6223	4.3299	0.1032 min	0.020 %
3	5.68 min	1830.0001	22039.3817	0.1785 min	99.945 %
4	21.90 min	0.5687	4.7612	0.1257 min	0.022 %